

**NIST**  
National  
Institute of  
Standards  
and Technology


*...working with industry to develop and apply technology, measurements and standards*

## Typing Single Nucleotide Polymorphisms (SNPs) Located on the Y Chromosome and in the Mitochondrial Genome

**NIST Division Seminar**  
October 16<sup>th</sup> 2003  
**Peter M. Vallone**  
DNA Technologies Group


### Overview

- SNPs
- Assay Platforms and Instrumentation
- Multiplexing
- U.S. Population Samples
- Y Chromosome and Mitochondrial Markers
- Results
  - mtSNP 11 plex
  - Y-SNP multiplexes



## SNP

### Single Nucleotide Polymorphism



Low mutation rate  $10^{-8}$   
Typically Biallelic

## SNP Facts

Most common type of variation in the human genome  
(90%)

Estimated to occur every 100-300 bases

For a SNP to be defined it must occur in at least 1 % of  
the population

2 out of every 3 SNPs is a C-T transition

Occur in coding and non coding regions of the genome

[http://www.ornl.gov/TechResources/Human\\_Genome/faq/snps.html](http://www.ornl.gov/TechResources/Human_Genome/faq/snps.html)


## Biomedical Importance of SNPs

Variations in DNA sequence can have a major impact on how humans respond to **disease, bacteria, viruses, toxins,**

According to a Frost & Sullivan report - "U.S. SNP Detection Technology Market," the market share of the diagnostics segment will grow from 11% in 2001 to 33% by 2009.

The report stated that the total SNP detection market generated \$91.28 million in 2001. This market is estimated to reach \$310.76 million by 2008.

from generation to generation --making them easier to follow in population studies



## Forensic Utility of SNPs

Human identification purposes (criminal, **paternity,** evolutionary, population studies, **predicting ethnicity**)

The short PCR amplicons required for typing SNPs may result in success with **degraded samples** and possibly higher sensitivity

Simplicity in testing – typically bi-allelic markers (versus length polymorphisms)

---

Improve assay development (both multiplex PCR and SNP detection)

For serious forensic usage parallel high-throughput methods will be required for typing

## Forensic Utility of SNPs

Short tandem repeat (STR)  
CTGATGCTA(**GATA**)<sub>n</sub>GACTACTTA  
n = 5 to 15 = 66 possible allelic combinations

SNP  
CTGATGCTA(**G/A**)GACTACTTA  
3 possible allelic combinations

For human ID purposes more  
SNPs would be needed than STRs  
Multiplexing is essential

## Overview

### SNPs

Assay Platforms and Instrumentation

Multiplexing

U.S. Population Samples

Y Chromosome and Mitochondrial Markers

Results


mtSNP 11 plex

Y-SNP multiplexes




## Instrumentation

PCR & primer extension




Multi-Color Capillary Electrophoresis  
(ABI 310 or 3100)

Luminex Beads hybridization




Luminex 100 Flow Cytometer



Primer Extension

Time-of-Flight Mass Spectrometer

TaqMan



ABI 7000 SDS

## Allele-Specific Primer Extension (ASPE)


Primer is extended by one base unit

ABI PRISM® SNaPshot™  
Multiplex System

Fluorescently labeled ddNTPs + polymerase

“tail” used to vary electrophoretic mobility

Oligonucleotide primer 18-28 bases

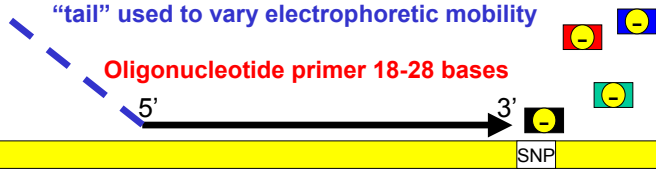

PCR Amplified DNA Template



ddNTP	Dye label	Color
A	dR6G	Green
C	dTAMRA	Black
G	dR110	Blue
T	dROX	Red

25 Cycles

96°C 10s

50°C 5s

60°C 30s

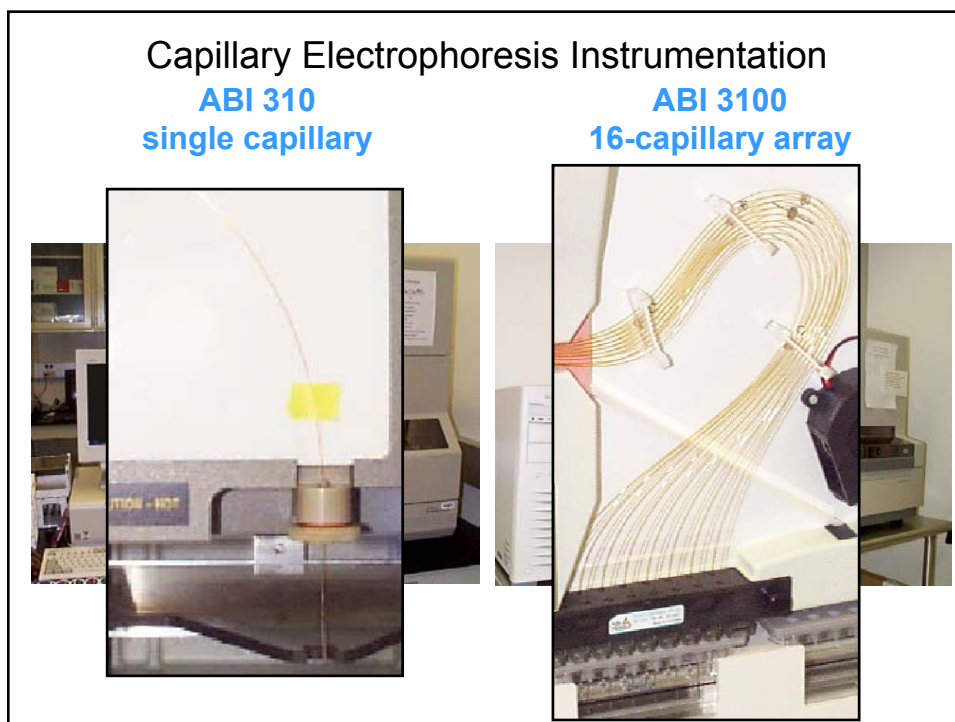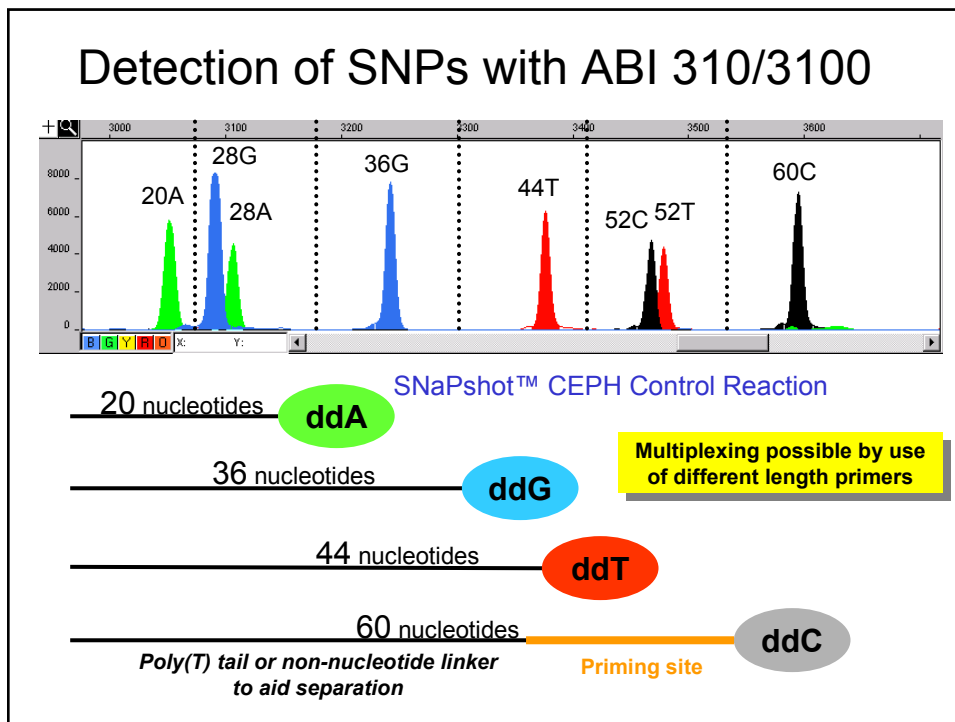

## SNP Detection by Hybridization

### Luminex Bead Array Assay

**Allele B**   **Allele A**

**PCR product**

100 different colored beads  
are possible (potential for  
multiplexing 50 SNP markers)

**Luminex 100 Flow Cytometer**

**Detects labeled  
PCR product**

**Identity of  
bead (probe)**

~30 seconds  
to process  
each sample

## ASPE combined with MALDI-TOF-MS Analysis

Primer is extended by one base unit

**Oligonucleotide primer 18-28 bases**

Natural non-labeled  
ddNTPs +  
polymerase

5'  3'

SNP

**PCR Amplified DNA Template**

ddNTP	Mass (Da)
A	297
C	273
G	313
T	288



40 Cycles

96°C 10s



50°C 20s

72°C 30s

Mass difference  
between SNP primer  
and single base  
extension product  
provides genotype

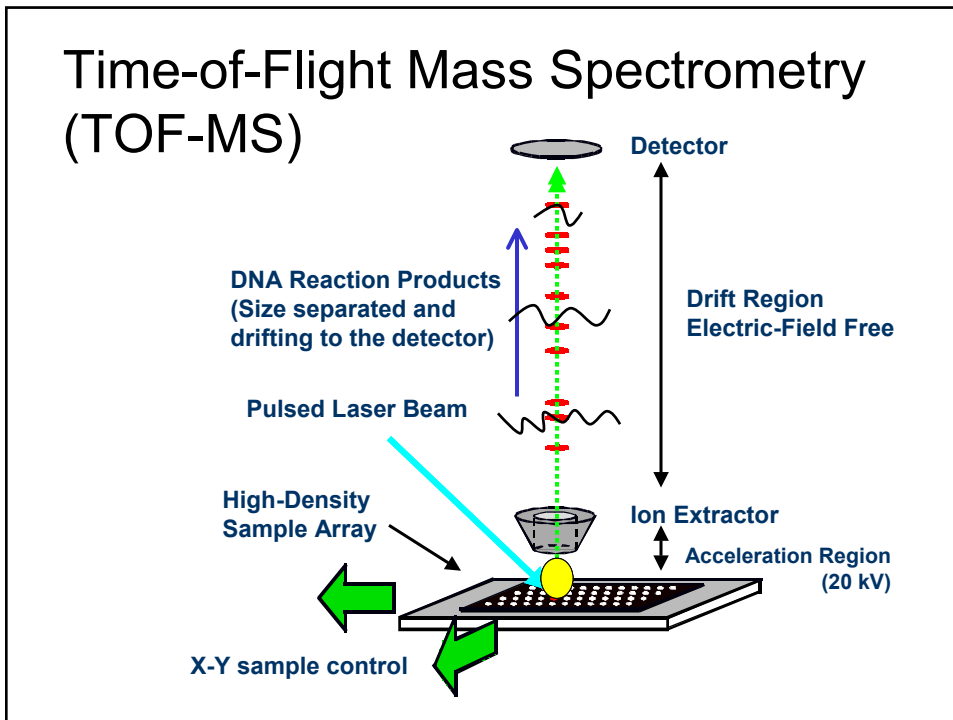



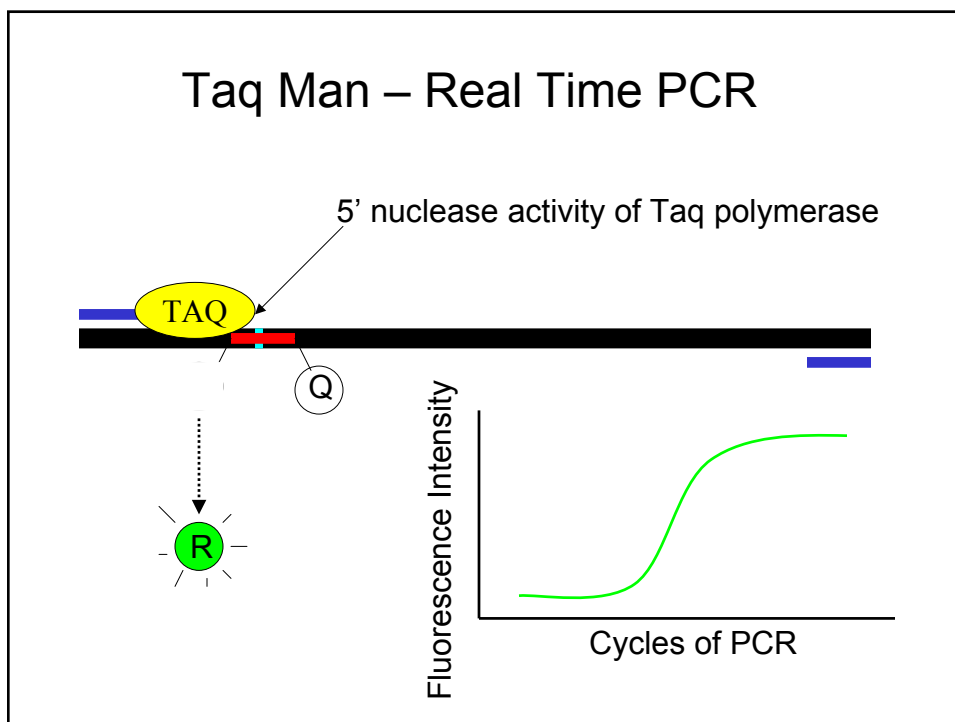

## Allelic Discrimination Assay using TaqMan

Design 2 Taqman probes for each expected SNP  
Each probe will have a different reporter dye (FAM/VIC)

Possible assays outcomes

SNP A = FAM

SNP B = VIC

SNP A/B = FAM/VIC



Typically TaqMan genotyping assays are singleplex!

## Summary of SNP Assays

	Advantages	Disadvantages
ASPE-CE	Moderate degree of	Development of multiplex
ASPE-M	Chip Based – Affymetrix - Agilent Allele specific PCR Invader-mismatch cleavage	multiplexing nt than CE
Microbe (Lumine)	Orchid SNPstream Illumina Bead Arrays	custom
TaqMan	Rapid - one step Good for one marker on 1000's of sample	No multiplexing Costly for typing many SNPs & few samples

## Overview

SNPs

Assay Platforms and Instrumentation

Multiplexing

U.S. Population Samples

Y Chromosome and Mitochondrial Markers

Results

mtSNP 11 plex

Y-SNP multiplexes



## Advantages of Multiplexing

Obtain more information per unit time

Reduce the amount of limited forensic sample used

Save on reagents; enzyme, buffers, DNA oligomers

Reduces labor

Streamlines data analysis

For certain markers it is essential (SNPs, YSTRs)

Coincides with high capacity instrumentation and new SNP typing technologies

## Goals for Multiplex Assay Development

Working with collaborators who have markers of forensic interest

Evaluate the forensic utility of newly discovered markers (medium sized multiplexes 5 – 10 loci)

Further the understanding of developing multiplex assays (primer design, QC)

Publish assay details for others to evaluate (commercial and research)

## Multiplex PCR Primer Selection

Identify markers of interest (collaborations, literature, research)

Organize sequences with ~250 bases of sequence up- and downstream of the SNP

PCR product size

Short amplicons for degraded samples, SNPs

Longer amplicons for STRs

Use software for selecting singleplex primer pairs

**Primer3**

[www-genome.wi.mit.edu/genome\\_software/other/primer3.html](http://www-genome.wi.mit.edu/genome_software/other/primer3.html)

Steve Rozen and Helen J. Skaletsky (2000) Primer3 on the WWW for general users and for biologist programmers. In: Krawetz S, Misener S (eds) *Bioinformatics Methods and Protocols: Methods in Molecular Biology*. Humana Press, Totowa, NJ, pp 365-386



## Format of Template Sequences

Locus	Total Length	Minimum	Maximum	Optimal	Excluded Region	SNP site
M3	255	105	150	125	174,60	204
TGATTATTTAGAAACAAAACAATAAACAATAACAAAACAATGGTTCCTGTAAAATGTC						
M9	255	105	150	125	237,60	267
CCTGTGCACGCCAAAGCGGAAGCTGAAGTGCGGCGTCTTTGATCTCTCAATCCTGGAG						

Sequences stored in excel  
Will be adapted for FASTA format & comma delimited

**Primer3 formatting program**

Primer3 Parameters

Desired Tm Range for PCR Primers

Minimum	Maximum	Optimum	Max Tm Difference
57	63	60	12.0

Desired Size Range for PCR Primers

Minimum	Maximum	Optimum
18	27	20

Primers to Return: 2

Set Parameters

Formats Primer3 parameters

Max 3' Stability: 9.0

Max 3' Mispriming: 12.0

Pair Max Mispriming: 12.0

Primer GC%: 20.0 - 80.0

Max Self Comp: 8.0

Max 3' Comp: 3.0

Max # N's: 0

Max Poly-X: 3.0

Ct (nM): 50.0

Salt Conc (mM) - KCl: 50.0

Example input  
format for  
Primer3

```

PRIMER_SEQUENCE_ID=M9
SEQUENCE=GCAGCATATAAACTTTCAGGACCCTGAAATACAGAAGCTG
CAAAGAAACGGCCTAAGATGGTTGAATNCTCTTTATTTTCTTTAATTTAG
ACATGTTCAAACGTTCAATGTCTTACATACTTAGTTATGTAAGTAAGGTAG
CGCTTACTTCATTATGCATTTCAATACTCAAAAAAATTCCTTTGTGAAAT
GTTGAAATATTTTCTAATCTGTTTCACGAGCTTCAAAAATGAGGAAAAA
GATTCAGTTTACATTTACGAAAATGCCTCTTTTAATCGGATTTATGTTT
ACTTAACATTTACAGTACATTTACGCTTGAGCAAAGTTAGGTTTT
PRIMER_COMMENT=(340 bp); G to C at position 68
PRIMER_MISPRIMING_LIBRARY=/Users/vallone/Desktop/primer3/misprM9
PRIMER_MAX_MISPRIMING=8
PRIMER_PAIR_MAX_MISPRIMING=20
EXCLUDED_REGION=38,60
PRIMER_PRODUCT_SIZE_RANGE=90-150
PRIMER_PRODUCT_OPT_SIZE=105
PRIMER_MIN_SIZE=18
PRIMER_MAX_SIZE=27
PRIMER_OPT_SIZE=20
PRIMER_OPT_TM=60
PRIMER_MIN_TM=57
PRIMER_MAX_TM=63
PRIMER_NUM_RETURN=1
PRIMER_EXPLAIN_FLAG=1
PRIMER_LIBERAL_BASE=1
=
PRIMER_SEQUENCE_ID=M42
SEQUENCE=AAAGCGAGAGATTCAATCCAGGATGACAGAATGCGTTCAC
CTTTAAAGGGATTAAGAAGTATAATACAGTCTGTATTATTAGATCACCC
AGAGACACACAAAACAAGAACCCTGAATTGAATTAGTGGTATACTAATAG
ACTGCTTTACCTGAAATATTTACAGATCAATGCTACTGAAATTTCTTACAG


```

## Non-Specific Interactions

Primers that interact with non-specific (undesired) regions of a genome OR with each other can degrade PCR performance

Screening for alternate genomic binding regions can be accomplished using **BLAST** <http://www.ncbi.nlm.nih.gov>

Screening for potential primer-dimer interactions is accomplished using in house software - **AutoDimer**

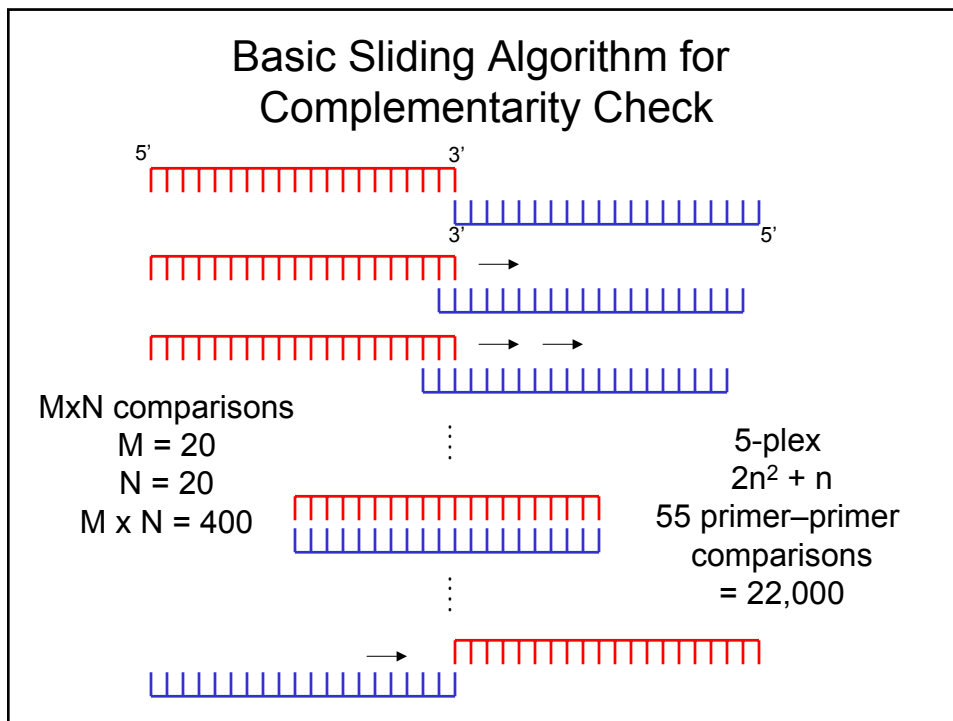

**Auto Dimer Check**

File Help About

Primer Dimer Checker

Cancel

Hairpin Checker

SAVE DATA

Minimum SCORE Requirement

6

# of Sequences

# of Hits: 22

253

Total Number of Primer-Primer Comparisons

Na+ (Molar)

0.085

Total Strand Conc (micromolar)

1.0

**AutoDimer**

$2n^2+n$

7202-F ACGCCAAAATCCATTTCAC T versus 16519-F ACCACCATCCTCCGTGAAAT

Matches = 7

Score = 6

ATTTCACN

est. tm = 3.6 oC

DeltaG @37 degrees = -3.85 kcal/mole

3' -TAAAGTGCCTCCTACCACCA-5'

|||||x

5' -ACGCCAAAATCCATTTCAC T-3'

10211-F ACCACAAC TCAACGGCTACA versus 3010-R TCACGTAGGACTTTAATCGTTGA


Matches = 9

Score = 6

TCACCGMTANA



## PCR Primer Quality Control



**6FAM** (yellow), **VIC** (orange), **NED** (red)

- **UV Spec** to determine concentration
- **HPLC** to evaluate purity
- **TOF-MS** to confirm correct sequence


Butler *et al.* (2001) *Forensic Sci. Int.* 119: 87-96

## Determination of DNA Oligomer Concentrations

	$\mu\text{M}$	% deviation	
Expected 100 $\mu\text{M}$	1	173.3	42.3
	2	164.8	39.3
	3	155.0	35.5
	4	124.1	19.4
	5	116.4	14.1
	6	98.5	-1.5
	7	108.6	7.9
	8	103.1	3.0
	9	120.8	17.2
	10	79.6	-25.7
	11	83.0	-20.5



Concentrations were estimated by UV Spec readings @260 using extinction coefficients determined from nearest-neighbor values

# Varian Helix DHPLC System




- Oligo QC
- Oligo Purification
- Fluorescent dye studies (excess dye removal)

Reverse phase ion exchange column  
Heated to 60°C  
UV detection




# MALDI QC of Commercial Oligos

Loss of Fluorescent dye



Vallone and Butler (Oct 2000) *International Symposium on Human Identification* (Biloxi, MS)



## Publications Describing Multiplex Assay Design

Schoske, R., Vallone, P.M., Ruitberg, C.M., Butler, J.M. (2003) Multiplex PCR design strategy used for the simultaneous amplification of 10 Y chromosome short tandem repeat (STR) loci. *Anal. Bioanal. Chem.*, 375: 333-343.

Butler, J.M., Schoske, R., Vallone, P.M. Highly multiplexed assays for measuring polymorphisms on the Y-chromosome. (2003) *Progress in Forensic Genetics 9* (Brinkmann, B. and Carracedo, A., eds.), Elsevier Science: Amsterdam, The Netherlands, International Congress Series 1239, pp. 301-305.

Schoske, R., Vallone, P.M., Kline, M.C., Redman, J.W., Butler, J.M. (2003) High-throughput Y-STR typing of U.S. populations with 27 regions of the Y chromosome using two multiplex PCR assays, *Forensic Sci. Int.*, in press

Butler, J.M. (2003) Constructing STR multiplex assays. *Methods in Molecular Biology: Forensic DNA Typing Protocols* (Carracedo, A., ed.), Humana Press: Totowa, New Jersey, in press.

Butler, J.M., Schoske, R., Vallone, P.M., Kline, M.C., Redd, A.J., Hammer, M.F. (2002) A novel multiplex for simultaneous amplification of 20 Y chromosome STR markers. *Forensic Sci. Int.* 129: 10-24.

Butler, J.M., David, V.A., O'Brien, S.J., Menotti-Raymond, M. (2002) The MeowPlex: a new DNA test using tetranucleotide STR markers for the domestic cat. *Profiles in DNA*, Promega Corporation, Volume 5, No. 2, pp. 7-10. [http://www.promega.com/profiles/502/ProfilesInDNA\\_502\\_07.pdf](http://www.promega.com/profiles/502/ProfilesInDNA_502_07.pdf)

Butler, J.M., Devaney, J.M., Marino, M.A., Vallone, P.M. (2001) Quality control of PCR primers used in multiplex STR amplifications. *Forensic Sci. Int.*, 119: 87-96.

Butler, J.M., C.M. Ruitberg, Vallone, P.M. (2001) Capillary electrophoresis as a tool for optimization of multiplex PCR reactions, *Fresenius J. Anal. Chem.* 369: 200-205.

## Overview

SNPs

Assay Platforms and Instrumentation

Multiplexing

U.S. Population Samples

Y Chromosome and Mitochondrial Markers

Results

mtSNP 11 plex

Y-SNP multiplexes



## NIST U.S. Population Samples

As of 08/2003 **666** males (anonymous; self-identified ethnicities)

260 Caucasians  
260 African Americans  
143 Hispanic  
3 Asian

Whole blood received from  
Interstate Blood Bank (Memphis, TN)

~80  $\mu\text{g}$  total extracted  
genomic DNA  
Working plates 1 ng/uL



To date: (35,139 allele calls)

Identifer (15 autosomal markers + Amelogenin) (10,608)

Roche Linear Arrays (HV1 HV2 10 regions) (6,630)

**Y-STRs 27 markers (17,901)**

## NIST U.S. Population Samples

As of 09/2003 **666 males** (anonymous; self-identified ethnicities)

- 260 Caucasians
- 260 African Americans
- 143 Hispanics
- 3 Asians

Whole blood received from Interstate Blood Bank (Memphis, TN)




Stock tubes



Working plates

Working tubes/plates 1 ng/uL



Working tubes

To date: (~50,000 allele calls)

Identifiler (15 autosomal markers + Amelogenin) (10,608)

Roche Linear Arrays (HV1/HV2 10 regions) (6,630)

Y-STRs 22 loci—27 amplicons (17,388)

Y-SNPs 50 markers on sub-set of samples (11,498)

Samples supplied to **OhioU** for miniSTR typing and **AFDIL** for whole mtGenome sequencing

## Overview

SNPs

Assay Platforms and Instrumentation

Multiplexing

U.S. Population Samples

Y Chromosome and Mitochondrial Markers

Results


mtSNP 11 plex

Y-SNP multiplexes



## Markers of Interest

- Mitochondrial DNA (mtDNA)
  - maternally inherited
  - polymorphic control region (D-loop)
  - ~500-2000 copies per cell
  - coding region



- Y chromosome
  - paternally inherited
  - variety of Y-STR and Y-SNP markers
  - ***haplotype rather than genotype***



Require large databases because recombination does not occur

## The Y Chromosome

60,000kb total size

The non-recombining region (NRY) consists of 95% of the Y chromosome

NRY is passed on as a block of information

Variations in the NRY are due to mutation only

Potential for predicting geographical origin



## Forensic Utility of Y Chromosome SNPs

Y chromosome markers are useful in mixed male - female samples

Haplogroups are non-randomly distributed among populations therefore potential exists for predicting population of origin

Low mutation rate of SNPs  $2e^{-8}$  per base per generation

The diagram shows a horizontal representation of the Y chromosome. It is divided into three main sections: a left pseudoautosomal region (orange), a central q arm (white), and a right pseudoautosomal region (orange). The q arm is further divided into a heterochromatin region (cross-hatched) and a region containing >250 Y-SNPs (white). Labels 'p' and 'q' are placed above the left and right arms respectively. Below the diagram, the text '>250 Y-SNPs described' is centered.

The image shows a complex phylogenetic tree of the Y chromosome. A red line traces a path through the tree, highlighting several key SNPs: M42(A/T), M168(C/T), M89(C/T), M9(C/G), M207(A/G), P25(C/A), and R1b. Each SNP is highlighted in a yellow box. The tree branches out to represent different haplogroups.



The Y Chromosome Consortium Map (2003)  
Nat Rev Genet. 4 :598-612

Tree contains over 250 Y-SNPs

Samples were typed for 48 world populations


18 main groups A-R

159 haplogroups defined

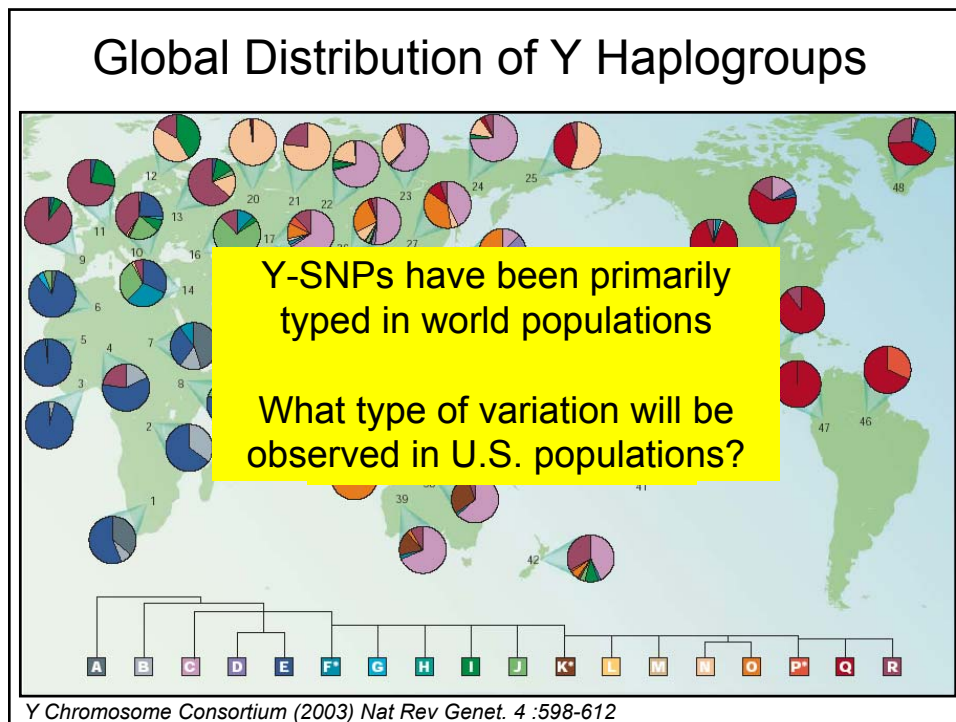



## The Current mtDNA Amplification & Sequencing Strategy Focuses on the Hypervariable Regions of the mitochondrial genome HV1 and HV2



In Caucasians, approximately 7% of HV1 and HV2 sequences are identical

## The Use of Full mtGenome Polymorphisms

mtGenome sequencing data reveals numerous SNPs that can help distinguish Caucasians sharing common HV types (Tom Parsons and Mike Coble AFDIL) 241 mt genomes


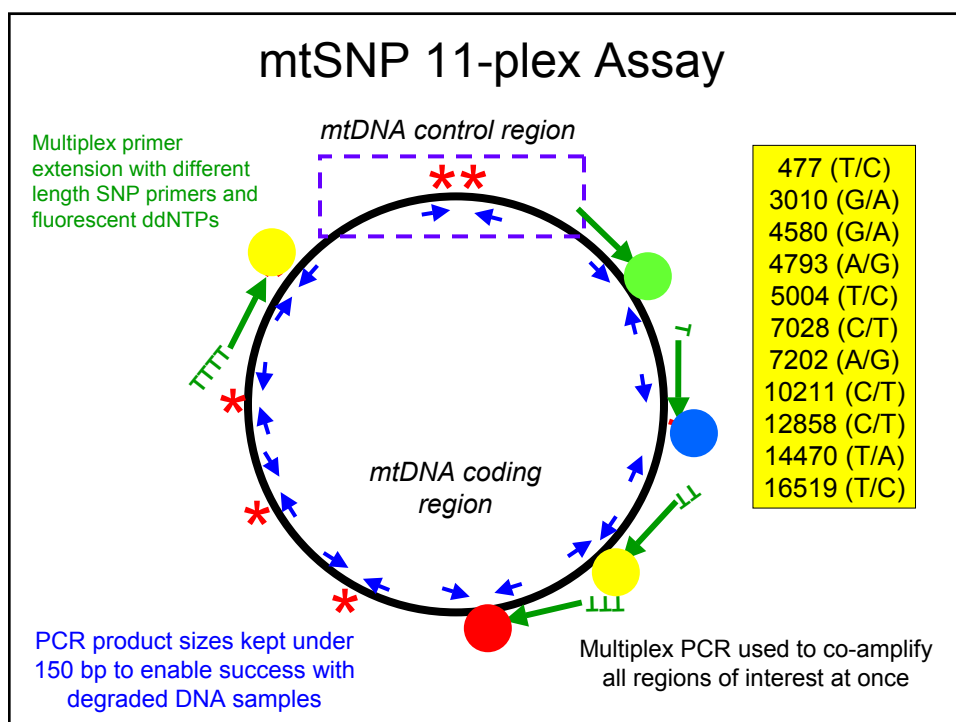
11 SNP sites were selected to help resolve Caucasian individuals having the most common HV1/HV2 type

mtSNPs: Silent and at third codon positions or fall in the short non-coding regions between genes in the coding region

Detect in a multiplex assay run on a common forensic instrumental platform

## Overview


- SNPs
- Assay Platforms and Instrumentation
- Multiplexing
- U.S. Population Samples
- Y Chromosome and Mitochondrial Markers
- Results
  - mtSNP 11 plex
  - Y-SNP multiplexes

## Tailed SNP primers allows for multiplexing in the SNaPshot assay

### Sequences for 11 extension primers

3010-F	TGTTGGATCAGGACATCCC	19 19
4793-R	(T) <sub>4</sub> – TCAGAAGTGAAAGGGGGC	18 22
10211-R	(T) <sub>10</sub> – ACTAAGAAGAATTTTATGGA	20 30
5004-F	(T) <sub>14</sub> – AGACCCAGCTACGCAAATC	20 34
7028-F	(T) <sub>18</sub> – GACACGTACTACGTTGTAGC	20 38
7202-F	(T) <sub>22</sub> – CCACAACACTTTCTCGGCCT	20 42
16519-R	(T) <sub>24</sub> – TGTGGGCTATTTAGGCTTTATG	22 46
12858-F	(T) <sub>27</sub> – GCAGCCATTCAAGCAATCCTATA	23 50
4580-R	(T) <sub>29</sub> – TGGTTAGAACTGGAATAAAAAGCTAG	25 54
477-F	(T) <sub>38</sub> – CCCTCCCCTCCCATACTAC	20 58
14470-R	(T) <sub>41</sub> – GGAATGATGGTTGTCTTTGG	21 62



### Program Output


Label	Length	Sequence	Position	Tm
Forward Primers Salt = 0.3Ct = 10				
M42 340 bp (A/T 297 W) AC010889	18	ATTTAGGACACAAAAGCW	280	60.65398
M42 340 bp (A/T 297 W) AC010889	19	GATTTAGGACACAAAAGCW	279	61.96716
M42 340 bp (A/T 297 W) AC010889	20	AGATTTAGGACACAAAAGCW	278	63.67808
Reverse Primers				
M42 340 bp (A/T 297 W) AC010889	23	GCTCTCTTTTTCATTATGTAGTW	319	63.5462
M42 340 bp (A/T 297 W) AC010889	21	TCTCTTTTTCATTATGTAGTW	317	59.28964
M42 340 bp (A/T 297 W) AC010889	20	CTCTTTTTCATTATGTAGTW	316	57.50257



Hairpin	Dimer	Template	Mass	Rank	Mutation	+ddC	+ddT	+ddA	+ddG
4	8	10	5273.48	2.133333	W	N/A	5561.67998	5570.68998	N/A
5	10	10	5602.69	2	W	N/A	5890.889941	5899.899941	N/A
5	10	11	5915.9	2	W	N/A	6204.099902	6213.109902	N/A
4	8	22	6734.42	2.133333	W	N/A	7022.619922	7031.629922	N/A
4	8	20	6116.02	2.133333	W	N/A	6404.22002	6413.23002	N/A
4	8	19	5811.82	2.133333	W	N/A	6100.019824	6109.029824	N/A



### mtSNP 11-plex run on ABI 3100

#### Multiplex PCR and Multiplex SNP Detection


Measured size (nt) (relative to GSLIZ-120 size standard)



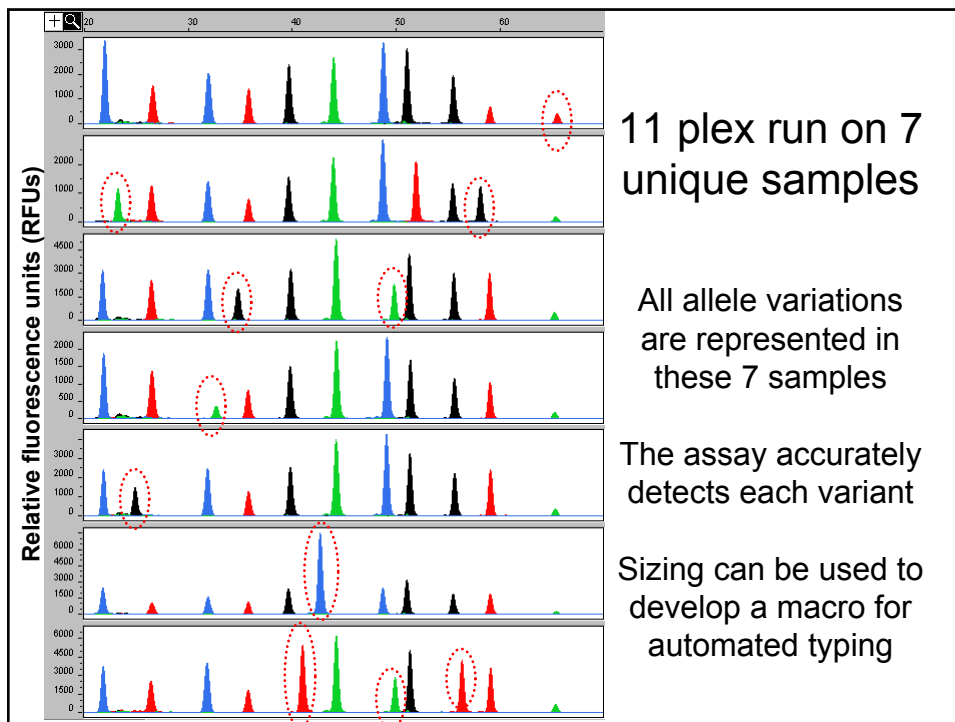

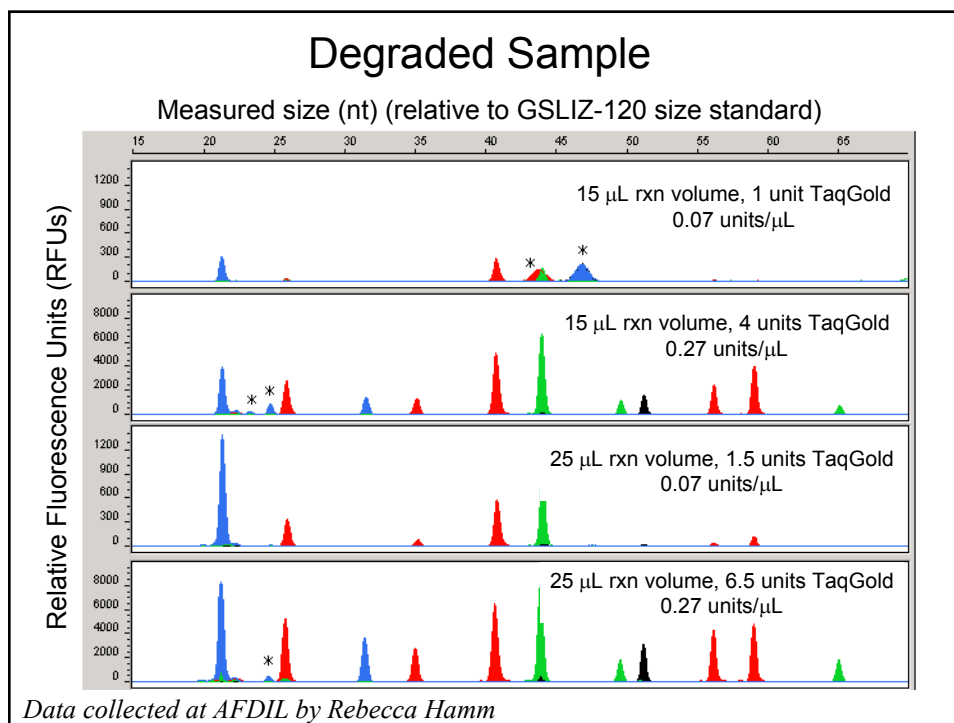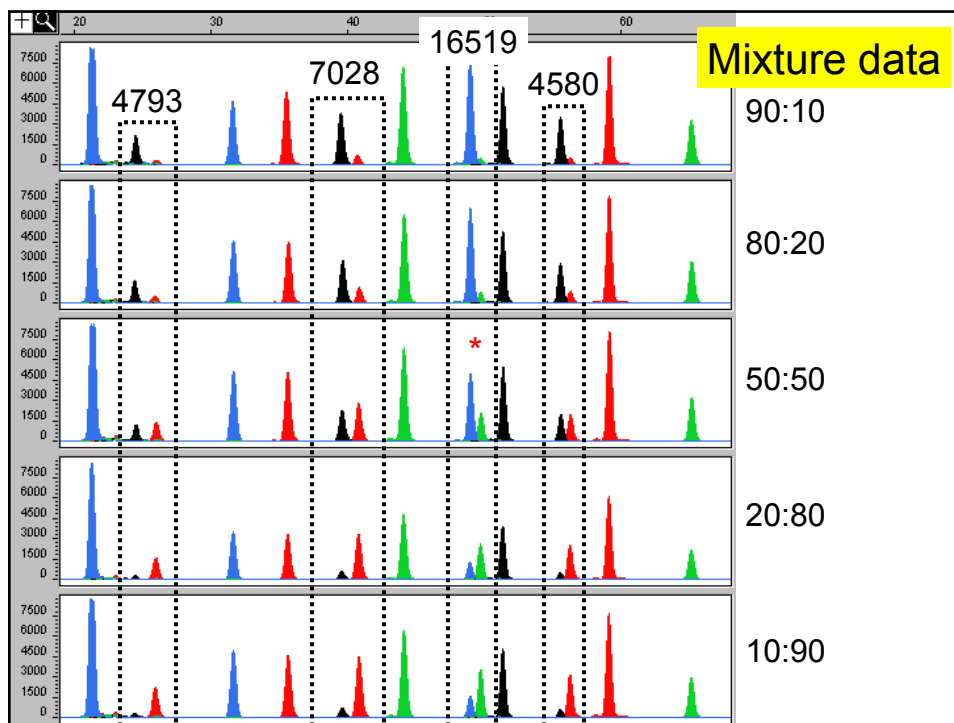

## Roche Linear Arrays

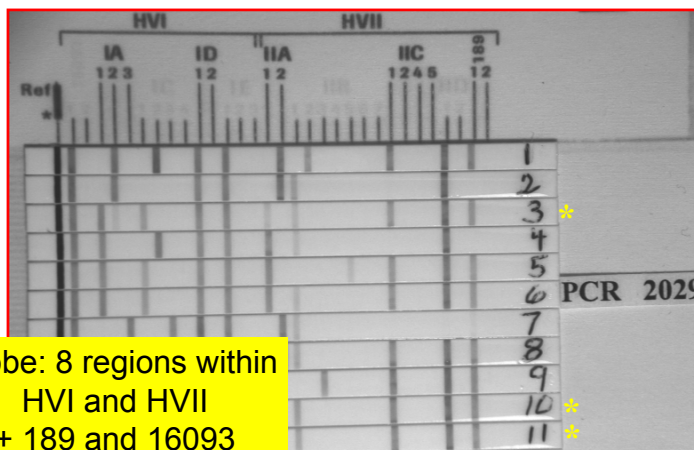

Probe: 8 regions within HVI and HVII + 189 and 16093 Run on all NIST U.S. population samples

Mito type 11111111AT U.S. Caucasian pop 47 / 286 = 16.4%

Data collected by Margaret Kline and Jan Redman

## Typing 51 samples with mt 11 plex assay

51 (47 cauc/4 hisp) samples were identical by Roche linear array assay (most common Haplogroup observed in NIST U.S. Caucasian population samples)

3010	G	A	G	G	G	A	G	G	G	G	G	G	A
4793	A	A	A	A	A	A	A	A	A	G	A	A	A
10211	C	C	C	C	C	C	C	C	C	C	C	C	C
5004	T	C	T	T	T	T	T	T	T	T	T	T	T
7028	C	C	C	T	C	T	C	T	C	C	C	C	C
7202	A	A	A	A	A	A	A	A	A	A	A	A	A
16519	T	C	T	C	T	C	C	T	T	C	C	C	C
12858	C	T	C	C	C	C	C	C	C	C	C	C	C
4580	G	G	G	G	G	A	G	A	G	G	G	G	G
477	T	C	T	T	T	C	T	T	T	T	T	T	T
14470	T	T	T	A	T	T	T	T	T	T	T	T	T
rCRS		1	1	1	1	2	2	3	4	4	5	12	15

12 haplogroups were observed  
4 haplogroups were unique  
2 of 11 sites did not vary

## 11-plex mtSNP assay

Assay is capable of accurately detecting 11 mtSNP in a single assay

The 11-plex assay is currently being validated for case work samples at AFDIL

Manuscript has been submitted

Additional multiplex mtSNP assays are being developed for other common HV1/HV2 types in collaboration with AFDIL

## Overview

SNPs

Assay Platforms and Instrumentation

Multiplexing

U.S. Population Samples

Y Chromosome and Mitochondrial Markers

Results

mtSNP 11 plex

Y-SNP multiplexes





## Y-SNPs in U.S. populations

What haplogroups will be observed?

How specific will certain Y-SNPs be for a U.S. population group?

Forensic utility in comparison/addition to Y-STRs

---

Commercial kit (Marligen) 42 Y-SNPs

Medium sized multiplexes developed in-house (CE or MS)

## Y-SNPs Typed at NIST

42 SNPs + Amelogenin present in 5 multiplexes  
(commercially available kit from Marligen)

18 SNPs in 3 NIST-designed 6plexes (8 unique)

10 SNPs in 2 NIST-designed 5plexes (1 unique)

19 of the SNP sites overlapped...



### **Resulting in a total of 51 Y-SNPs**

115 African Americans


114 Caucasians

95 Hispanics (presently typed for 10 Y-SNPs)



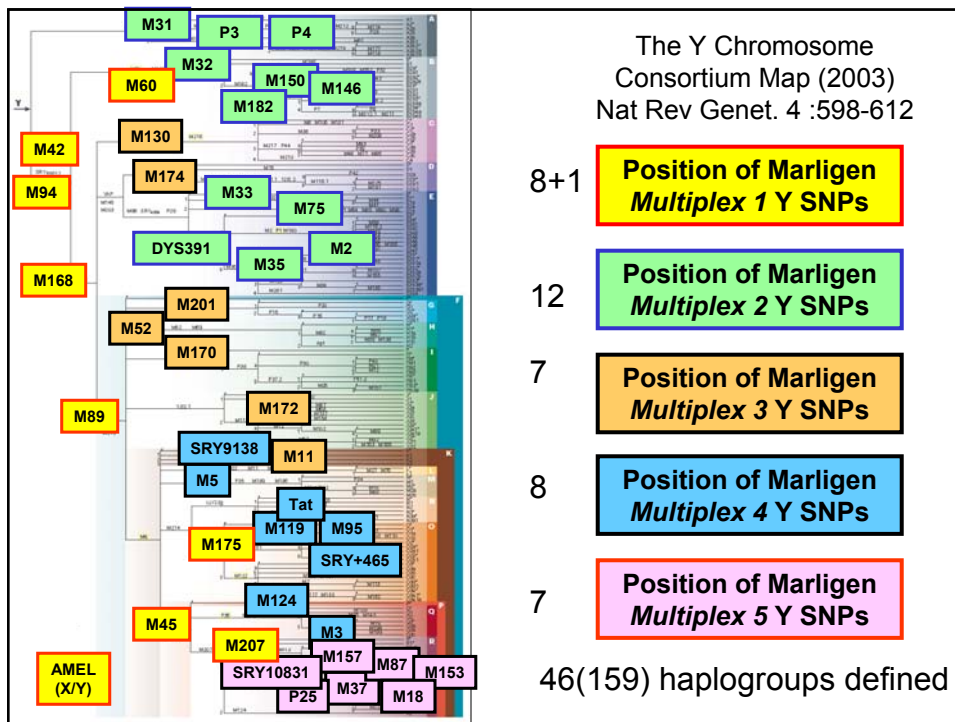

## ASPE Assays for 10 Y-SNPs



Equimolar PCR primer concentration (5plex)  
Empirical balancing of extension primers

## Summary of Y-SNP Data

(115 African Americans and 114 Caucasians)


A total of 20 ng of genomic DNA was consumed for the 10 multiplexes

18 out of 46 haplogroups observed

Over 99 % success rate for allele calls (both methods)

Variation was observed in 24 of the 51 Y-SNPs


100% concordance for the 18 overlapping markers (>3,800 allele calls)

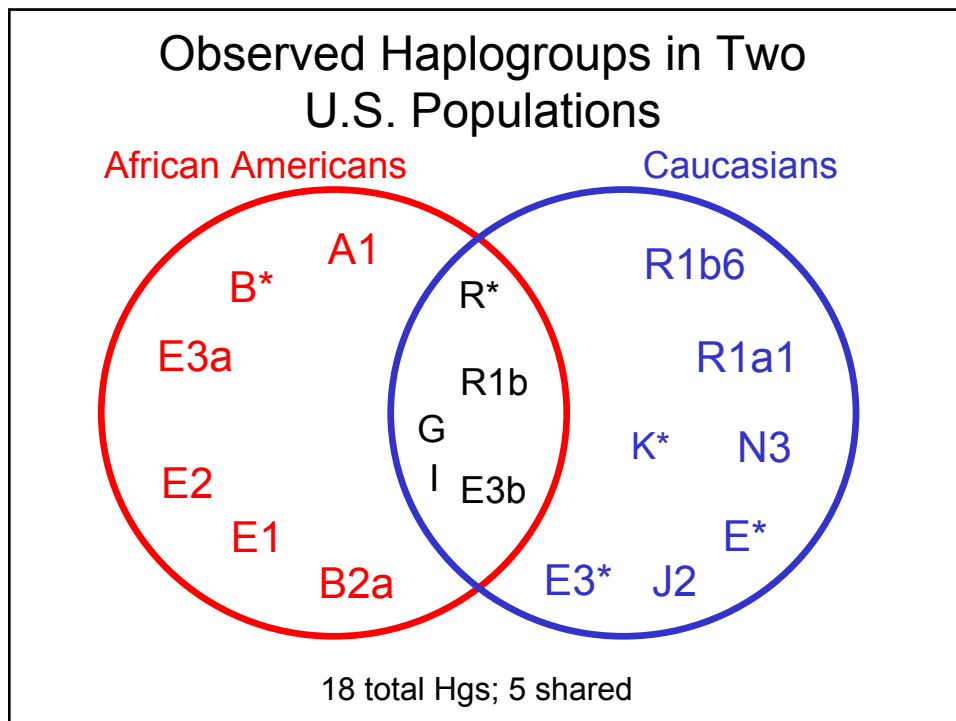

### Variation was not observed for 27 Y-SNPs (in AA and CAUC populations)


<u>M175 +/-</u>	<u>M119 A/C</u>	<u>M37 C/T</u>
<u>M146 A/C</u>	<u>M124 C/T</u>	<u>M87 T/C</u>
<u>M32 T/C</u>	<u>M3 C/T</u>	<u>M69 T/C</u>
<u>P3 (C/T)</u>	<u>M5 C/T</u>	<u>M112 G/A</u>
<u>P4 (G/A)</u>	<u>M95 C/T</u>	<u>M122 T/C</u>
<u>M11 A/G</u>	<u>SRY465 C/T</u>	<u>M123 G/A</u>
<u>M130 C/T</u>	<u>SRY9138 C/T</u>	<u>M137 T/C</u>
<u>M174 T/C</u>	<u>M157 A/C</u>	<u>M166 G/A</u>
<u>M52 A/C</u>	<u>M18 +/-</u>	<u>P36</u>



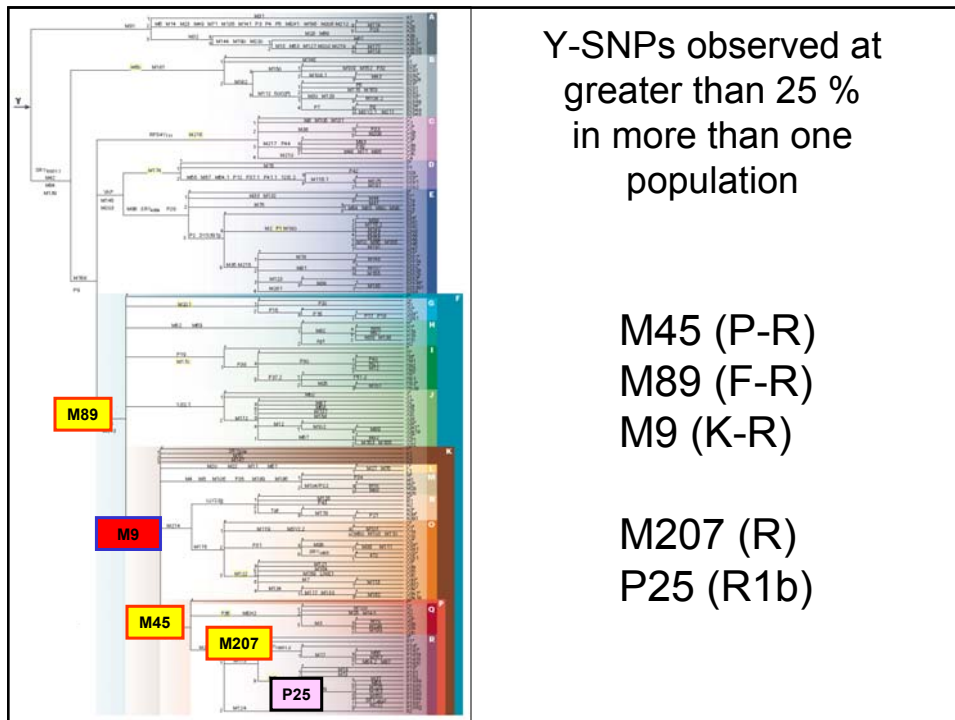



### Derived in more than one population

Locus	All	AA	Cauc	Hisp	Hap
<u>M2 A/G</u>	0.23	0.58	not obs	0.08	E3a
<u>DYS391 C/G</u>	0.31	0.60	0.04	na	E3
<u>M170 A/C</u>	0.10	0.04	0.21	0.04	I
<u>M35 G/C</u>	0.02	0.02	0.03	na	E3b
<u>M201 G/T</u>	0.03	0.01	0.03	0.05	G
<u>SRY10831 A/G</u>	0.03	0.01	0.05	na	R1a

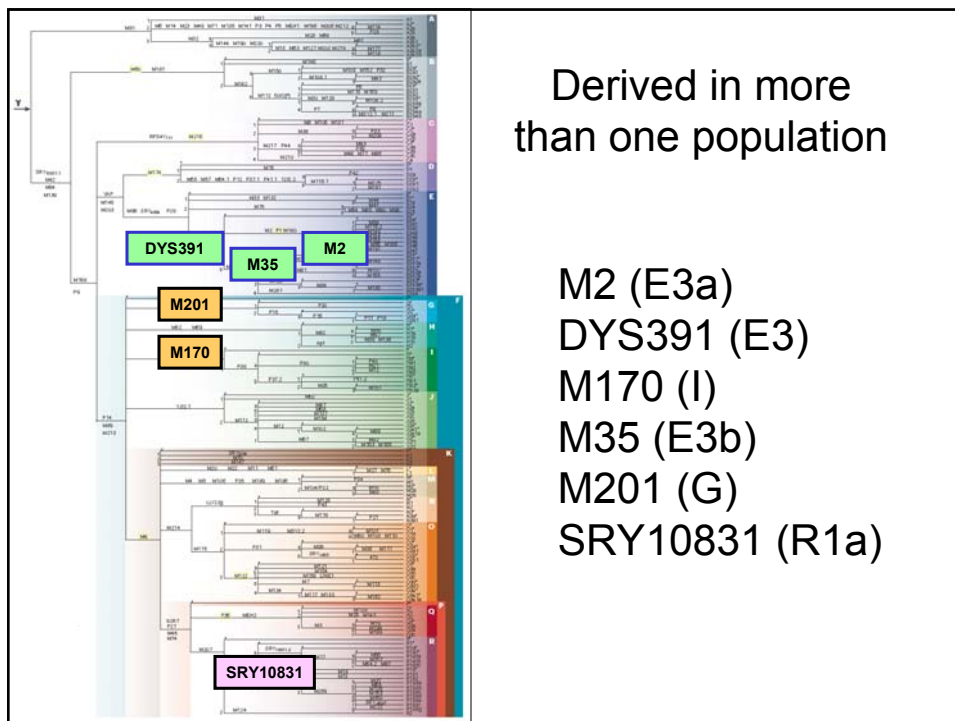


### Low frequency and population specific

Locus	All	AA	Cauc	Hisp
<u>M168 C/T</u>	0.01	0.03	not obs	na
<u>M42 A/T</u>	0.04	0.01	not obs	na
<u>M60 -/+</u>	0.01	0.02	not obs	not obs
<u>M94 C/A</u>	0.01	0.01	not obs	na
<u>M150 C/T</u>	0.01	0.01	not obs	na
<u>M182 C/T</u>	0.01	0.01	not obs	na
<u>M31 G/C</u>	0.01	0.01	not obs	na
<u>M33 A/C</u>	0.01	0.03	not obs	na
<u>M75 G/A</u>	0.01	0.03	not obs	na
<u>M172 T/G</u>	0.03	not obs	0.05	na
<u>M198 C/T</u>	0.03	not obs	0.05	na
<u>Tat T/C</u>	0.01	not obs	0.01	na
<u>M153 T/A</u>	0.01	not obs	0.01	na

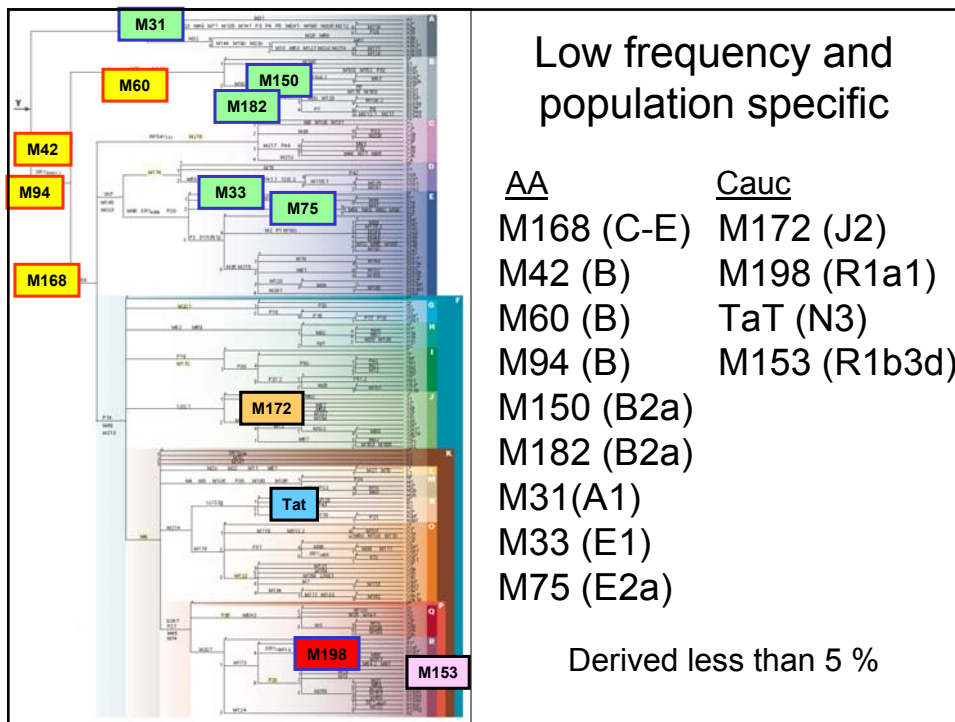







## Issues with Y-SNP P25


Initially when typing P25 with the Marligen kit the derived allele (A) was not observed

Alan Redd (Univ of AZ) informed us that P25 is a multi copy locus

After further review of our data we were able to make correct allele call for the P25 marker based on **signal intensity ratio**

BLAST results indicate that the region surrounding P25 is present 3 times on the Y chromosome

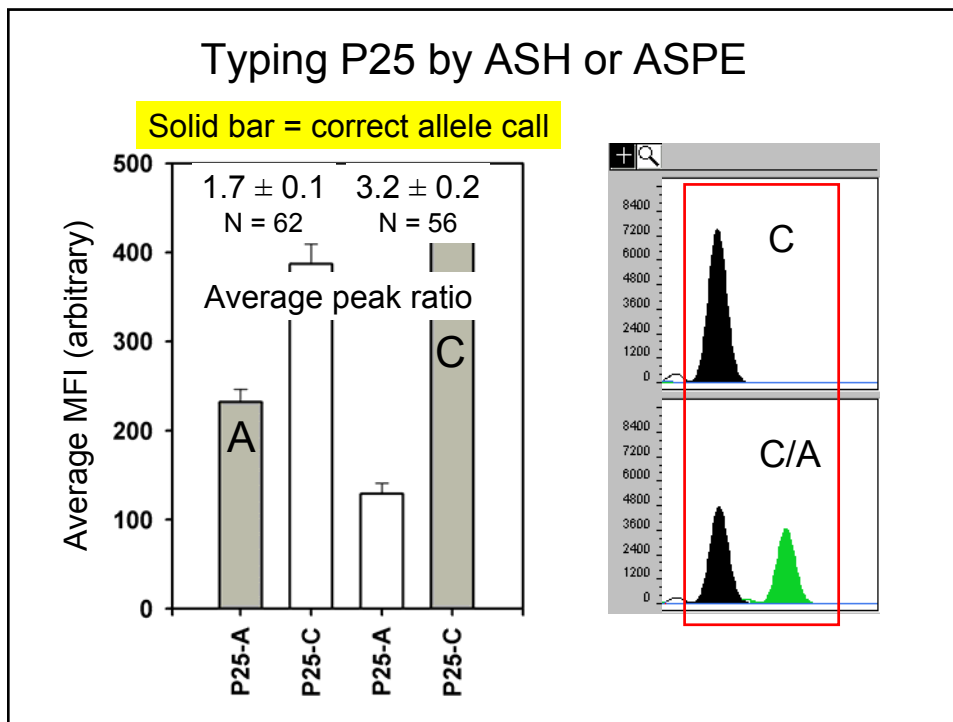



## Forensic Utility 51 Y-SNPs versus 1 Y-STR

For N = 211 male samples

	<u>51Y-SNPs</u>	<u>Y-STR DYS464</u>
Amount of sample consumed	10ng	1ng
Number for types observed	<b>18</b>	<b>62</b>
Analysis	Multiple	1 reaction
Degraded samples	+	?



## Y SNP Results on SRM 2395

SRM 2395	AMEL	M207 (A/G)	M45 (A/G)	M89 (C/T)	DYS391 (C/G)	M2 (A/G)	M170 (A/C)	M172 (G/T)	M201 (G/T)
Component A	XY	<b>G</b>	<b>A</b>	T	C	A	A	T	G
Component B	XY	A	G	T	C	A	A	<b>G</b>	G
Component C	XY	A	G	<b>C</b>	<b>G</b>	<b>G</b>	A	T	G
Component D	XY	A	G	T	C	A	A	T	<b>T</b>
Component E	XY	A	G	T	C	A	<b>C</b>	T	G
Component F	XX								

*SRM components are all distinguishable from one another with these Y SNPs*

*50 Y SNPs measured across all samples*

## Acknowledgments



### Funding:

**U.S. National Institute of Justice**

**Interagency Agreement between NIJ and NIST Office of Law Enforcement Standards**




John Butler

### Collaborators

**Thomas Parsons, Rebecca Hamm and Mike Coble (AFDIL)**  
**David Carlson (Marligen)**  
**Mike Hammer and Alan Redd (U of AZ)**

Jan Redman



Margaret Kline