


INTOXILYZER 8000 IMPLEMENTATION SCHEDULE

NOTE: All dates are subject to change. Please continue to check this web-site for additional information and revisions.

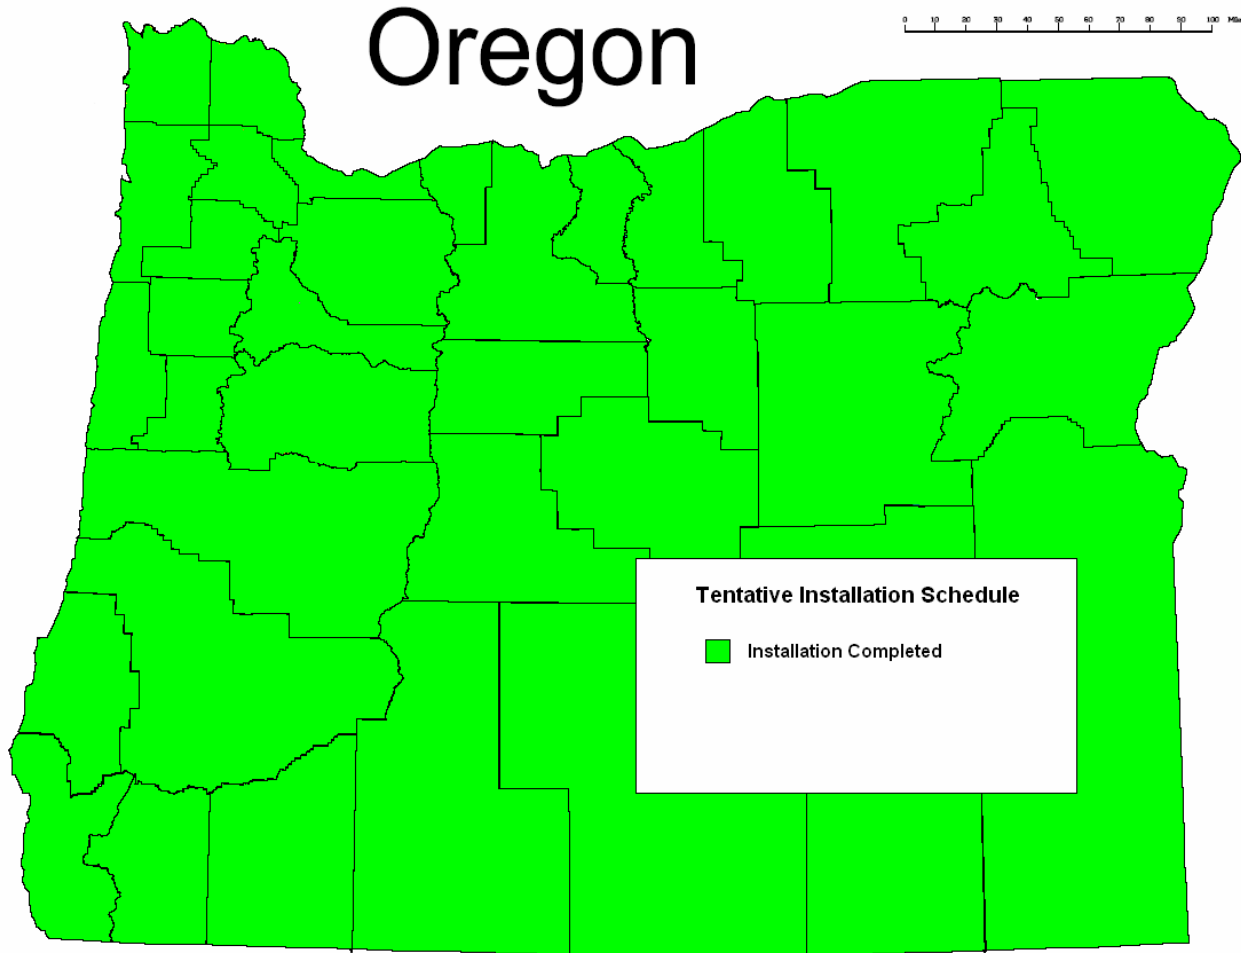

Please read below for additional information.

Agency Facility Requirements:

1. A minimum of two (2) square-feet to accommodate the instrument.
2. A minimum of two (2) square-feet to accommodate the external printer.
3. The instrument and the external printer must be located within three (3) feet of one another.
4. "C" sites only: Arrangements for dedicated modem lines will be paid for by the Oregon State Police; however, agencies will need to provide a physical address, a contact person and telephone number, and the name of the local telephone service provider to the Implied Consent Unit. Requests can be made directly to the Implied Consent Unit by calling (503) 451-2230.

Anticipated Implementation Schedule by County

*Date ranges are provided as approximate implementation "windows".

Date	County	Site(s)	# Sites
3/8/07	All counties	All sites have been installed	126