



Quality Assurance Site Information for Banning-Airport

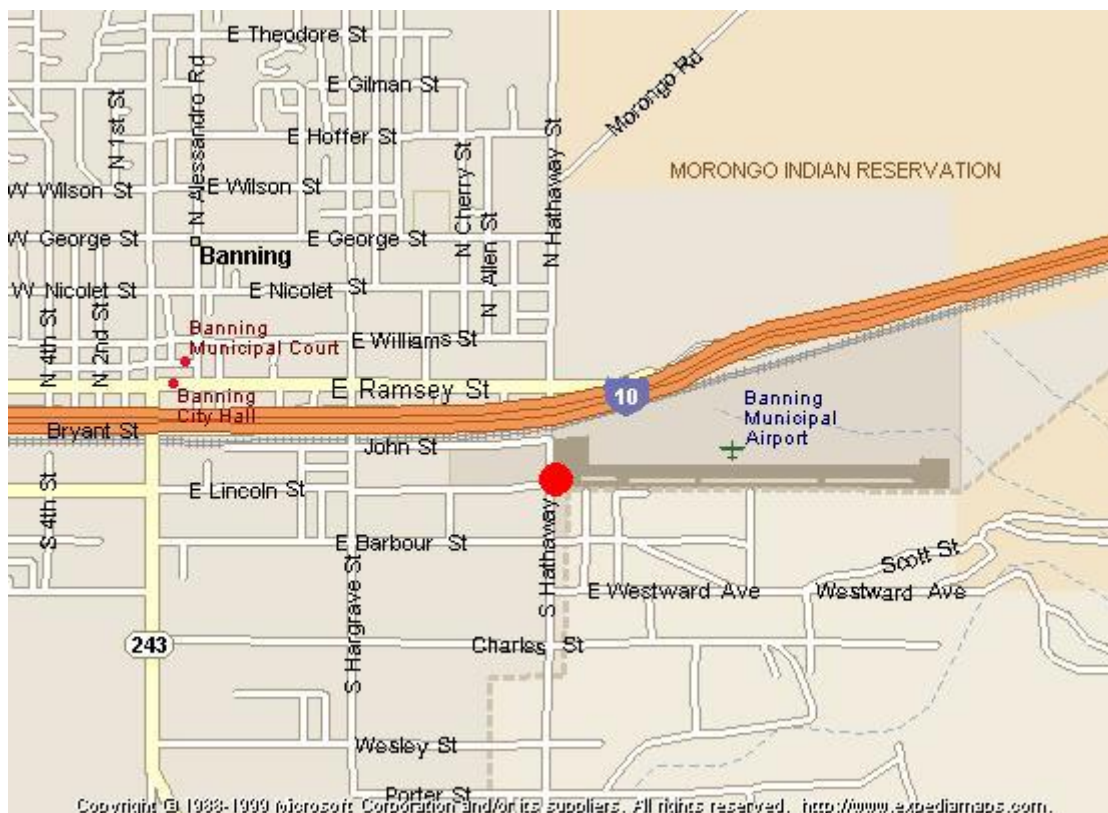

AIRS Number	ARB Number	Site Start Date	Reporting Agency and Agency Code
060650012	33164	04/01/95	South Coast AQMD (061)

Site Address	County	Air Basin	Latitude	Longitude	Elevation
200 S. Hathaway St, Banning CA 92220	Riverside	South Coast	33° 55' 15"	116° 51' 30"	473

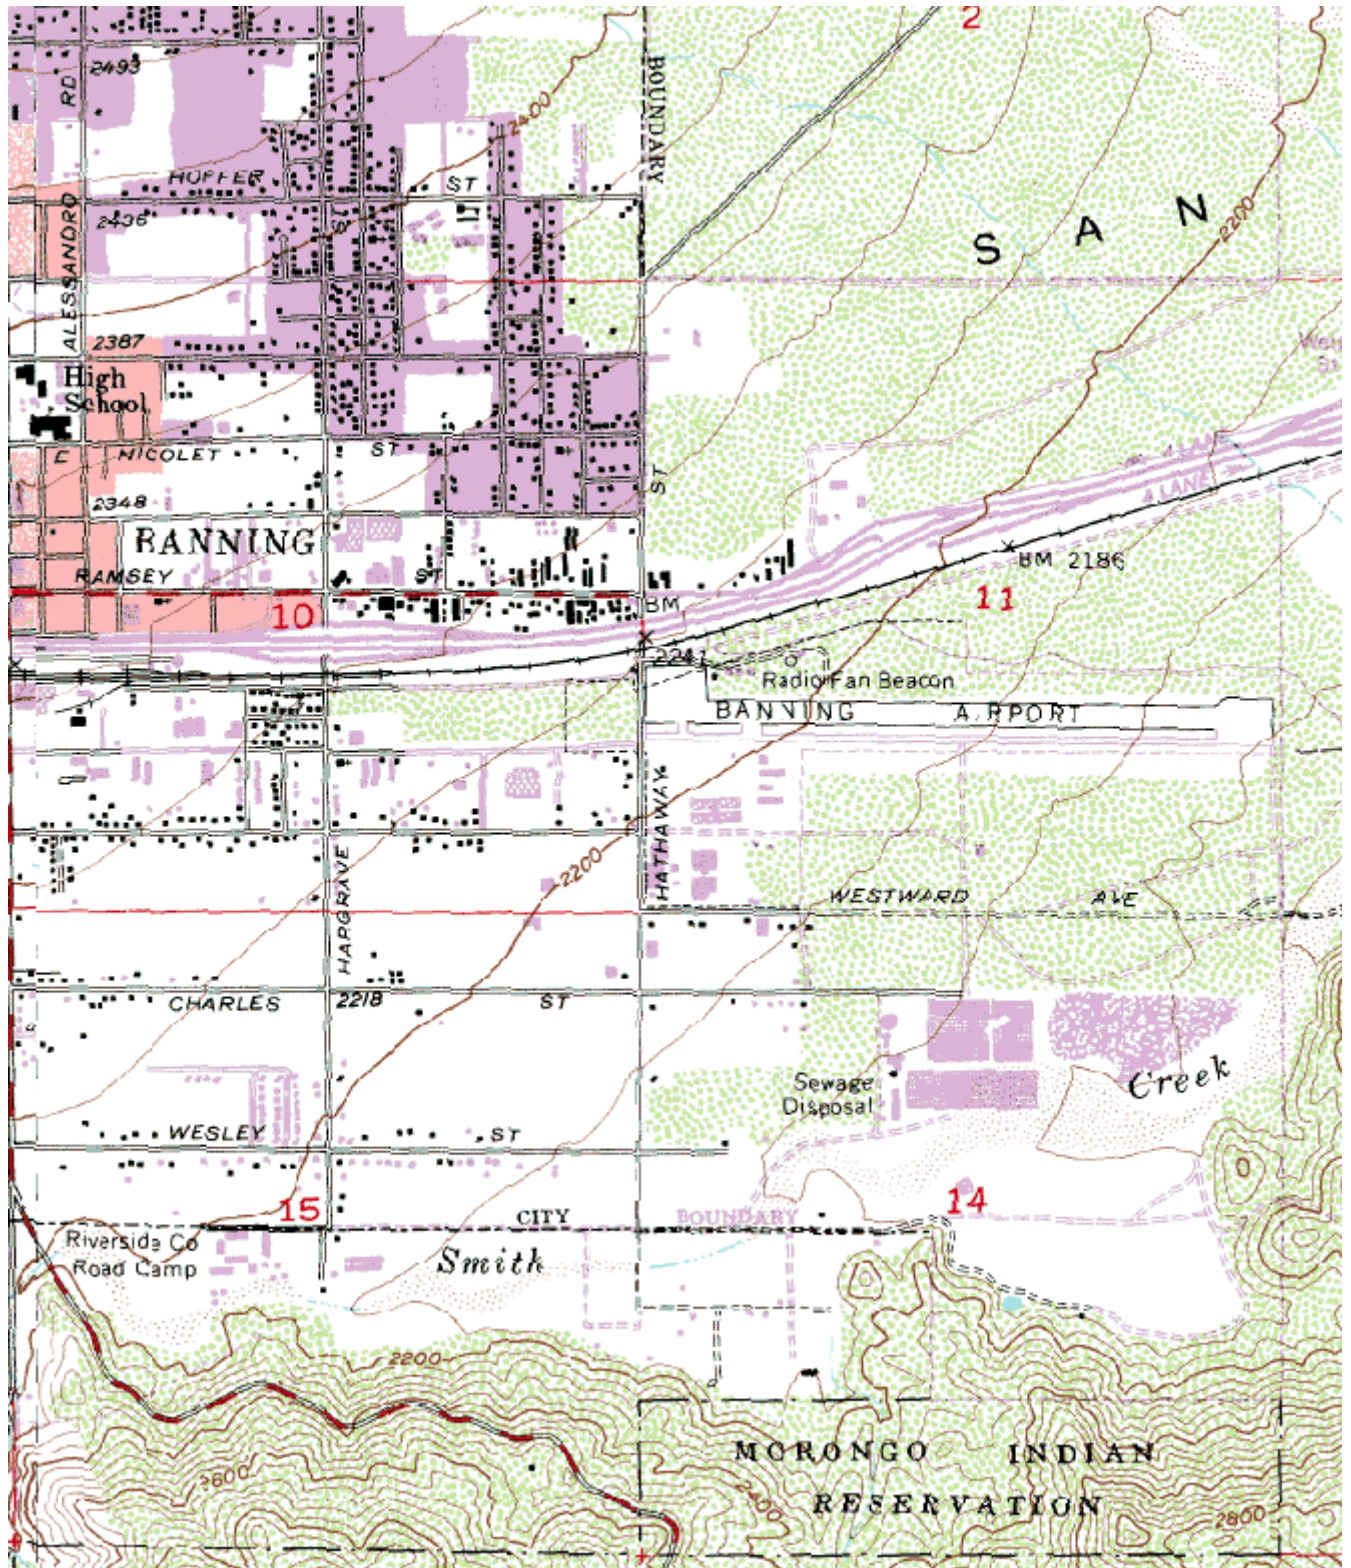

Site Survey Report

Siting Information

Site Name: Banning-Airport	Audit Date: 2006-08-10	ARB Number: 33164	AIRS Number: 060650012
Address: 200 S. Hathaway St Banning, CA 92220	Latitude: 33° 55' 15"	Longitude: 116° 51' 30"	Elevation (m): 473
	Auditors: Alvin Danque Long Liu	Site Technician: Richard Trzcinski	Site Phone:
Operating Agency: South Coast AQMD		Site Report: Yes	Site Photos: Yes

General Siting Conditions

Station Temperature Controlled: Yes Recorded: Yes Inside Temp: 25 Degrees Celsius	Traffic Description: Freeway Distance: 1000 meters Count (Veh/Day): 30000	Topography Site: level Region: Level	Predominant Wind Direction: East Arc Air Flow (Deg): 360 Degrees
		QA Manual Approved: Yes Agency: SCAQMD	Probe Clean: Yes
			Manifold Clean: Yes Cleaning Schedule: Annually
Meteorology Located With Instruments: Yes Shadowing: Yes Boom Orientation (Deg): n/a Temp(Motor/Natural): Natural	Non-vehicular Local Sources Description: aircraft Distance: 100 meters Direction: N/NE	Urbanization: Rural	Autocalibrator Type: Environics 100
		Ground Cover: Gravel	Site Survey Complete: Yes Logbook Up To Date: Yes

Site Survey Report (Cont.)

Monitor Type	Nitrogen Dioxide	Ozone	PM10-SSI
Manufacturer/Model	API 200	API/Teledyne 400	Sierra Andersen 1200
Serial Number	E000220	510	3546
POC	1	1	1
Data For Record?	Yes	Yes	Yes
Purpose			
Objective			
Scale			
Height Above Ground	4.2	4.2	2.5
Height Above Platform	1.5	1.5	1.5
Sampler Spacing			
Current Manual Available?	Yes	Yes	Yes
Instrument Log Up-to-date?	Yes	Yes	Yes
In-line Filter Change Date	2006-08-04	2006-08-04	
Cal. Gas Cert. Date	2005-11-09		
Calibration Current?	Yes	Yes	Yes
Calibration Date	2005-11-29	2006-05-23	2006-07-14
Cal. Equipment Cert. Date	2005-09-29	2005-09-29	2006-01-06
Obstacle Description	None	None	None
Distance to Obstacle	-	-	-
Height Above Inlet	-	-	-
Distance to Walls, etc.	-	-	-
Distance to Dripline	-	-	-
Dominant Influence	Vehicular	Vehicular	Vehicular
Residence Time (sec)	8.1	7.6	