



## Quality Assurance Site Information for Lake Elsinore-W Flint Street

*This page updated February 10, 2005*

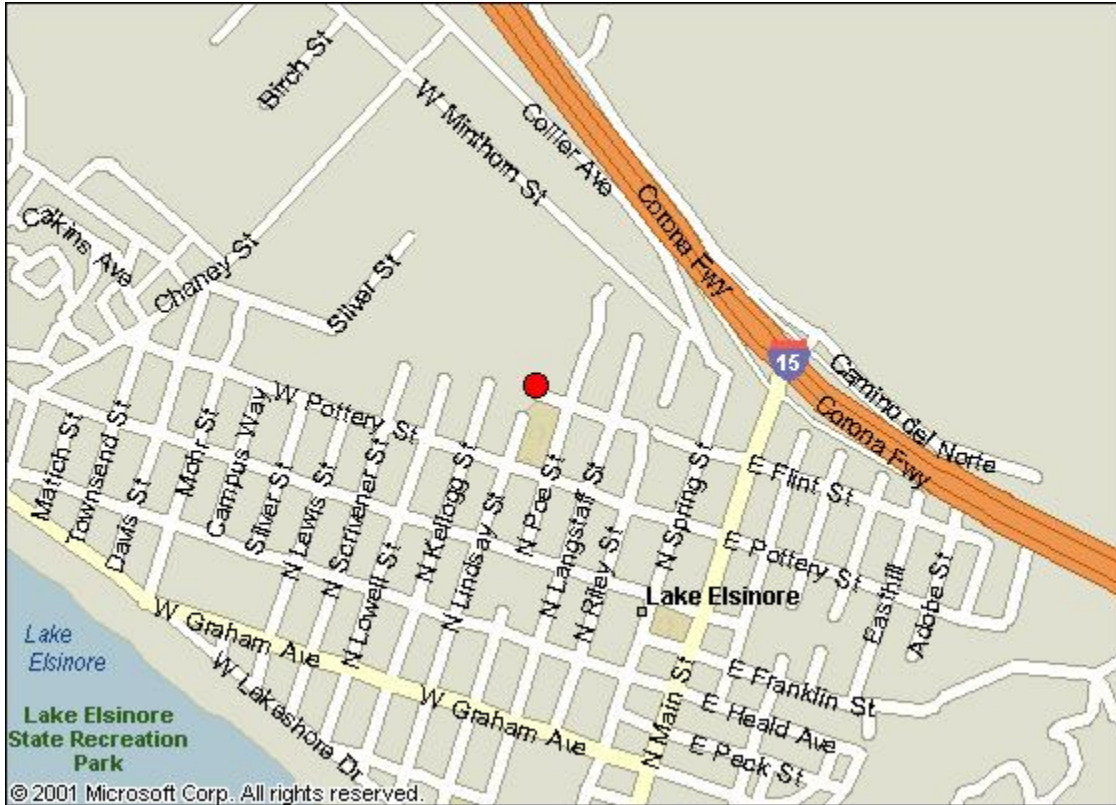

AIRS Number	ARB Number	Site Start Date	Reporting Agency and Agency Code
060659001	33158	10/1/88	South Coast AQMD (061)

Site Address	County	Air Basin	Latitude	Longitude	Elevation
506 W Flint Street, Lake Elsinore CA 92530	Riverside	South Coast	33° 40' 35"	117° 19' 51"	1449

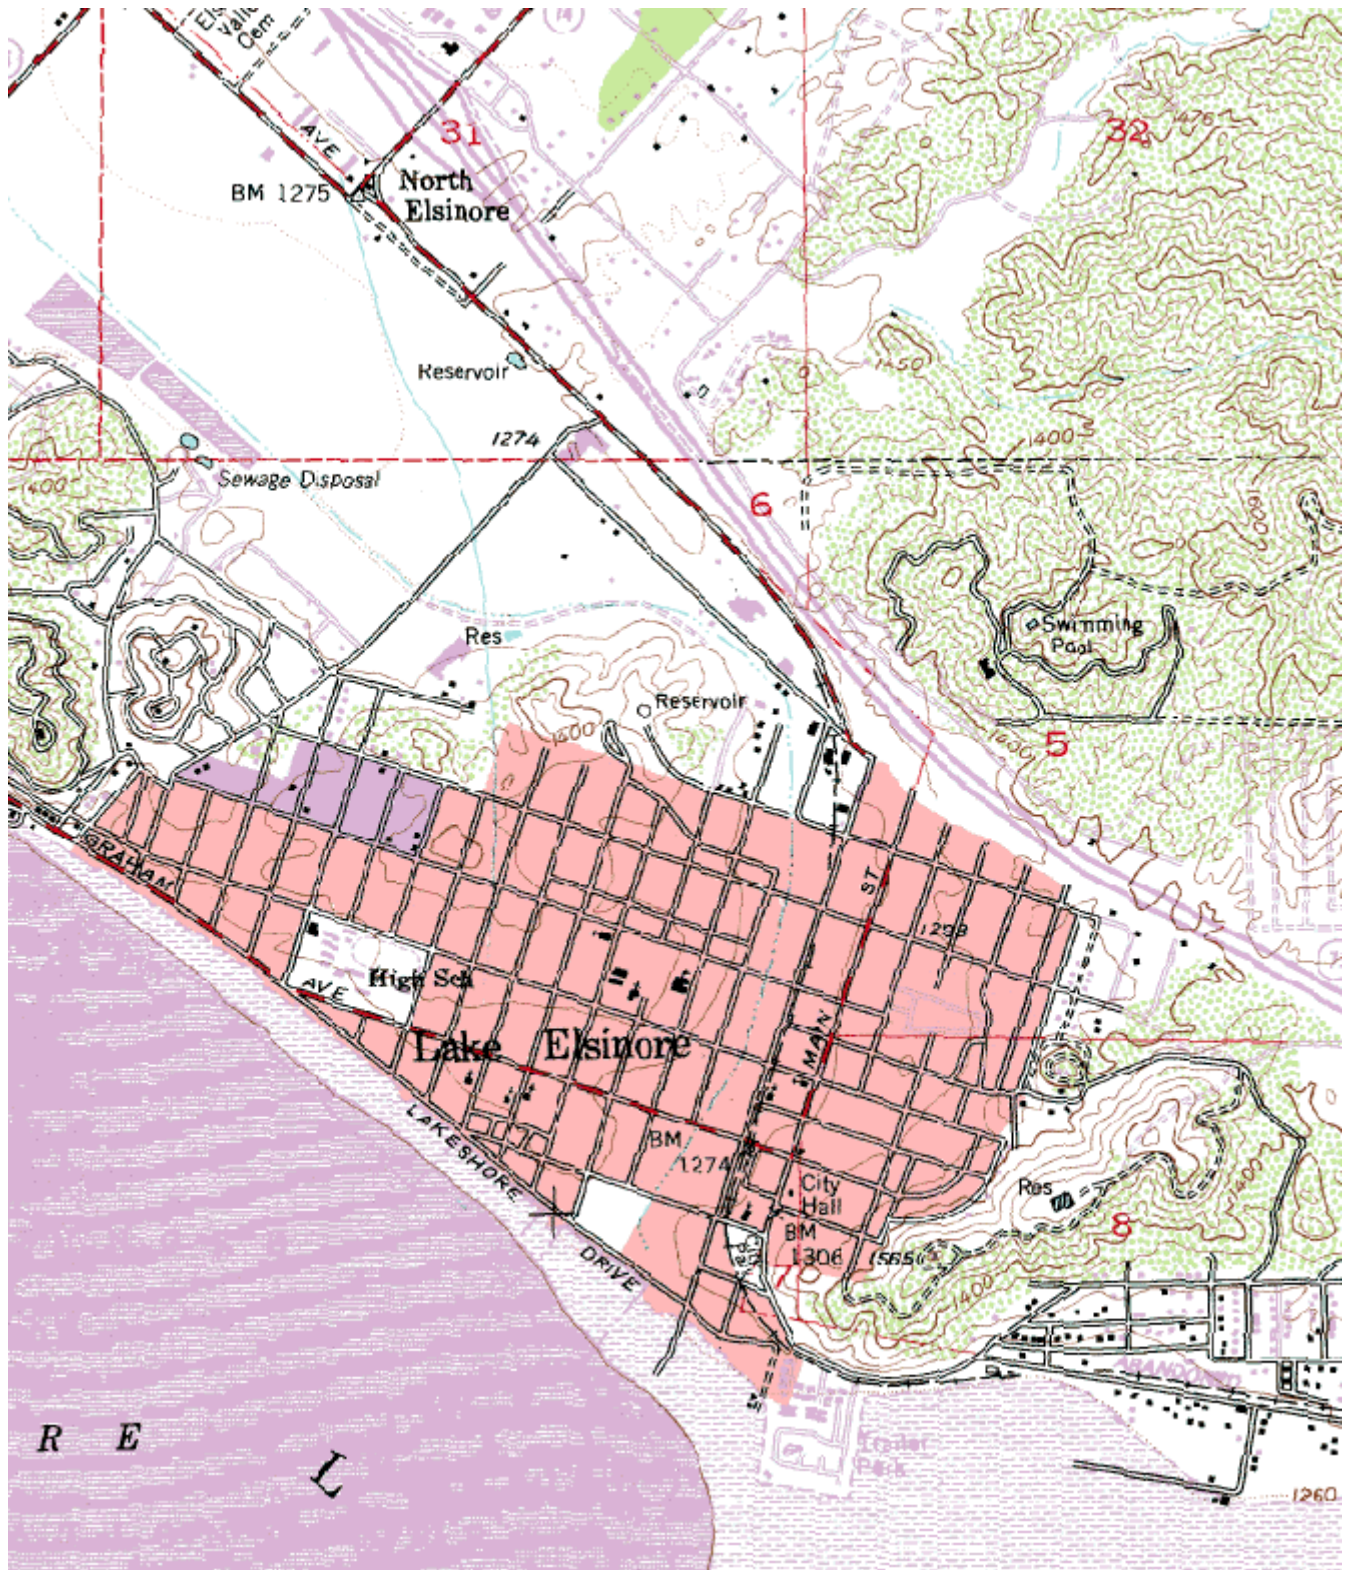

# Site Survey Report

## Siting Information

Site Name: Lake Elsinore-W Flint Street	Audit Date: 2006-08-03	ARB Number: 33158	AIRS Number: 060659001
Address: 506 W Flint Street Lake Elsinore, CA 92530	Latitude: 33° 40' 35"	Longitude: 117° 19' 51"	Elevation (m): 1449
	Auditors: Don Fitzell Alvin Danque	Site Technician: Mike Hamdan	Site Phone:
Operating Agency: South Coast AQMD		Site Report: Yes	Site Photos: Yes

## General Siting Conditions

<b>Station Temperature</b>  Controlled: Yes  Recorded: Yes  Inside Temp: 24 Degrees Celsius	<b>Traffic</b>  Description: Residential  Distance: 200 meters  Count (Veh/Day): 100	<b>Topography</b>  Site: Hilly  Region: Hilly	Predominant Wind Direction: South
			Arc Air Flow (Deg): 360 Degrees
		<b>Meteorology</b>  Located With Instruments: Yes  Shadowing: No  Boom Orientation (Deg): 345  Temp(Motor/Natural): Natural	<b>Non-vehicular Local Sources</b>  Description: construction  Distance: 25 meters  Direction: south
Agency: California Air Resources Board  Urbanization: Rural  Ground Cover: Dirt	Manifold Clean: Yes		
	Cleaning Schedule: Semi Annually		
	Autocalibrator Type: Environics 100		
			Site Survey Complete: Yes
			Logbook Up To Date: Yes

## Action Items

## Comments

## Site Survey Report (Cont.)

Monitor Type	Carbon Monoxide	Nitrogen Dioxide	Ozone	TEOM
Manufacturer/Model	Horiba APMA-360	API 200A	API/Teledyne 400	R&P 1400A
Serial Number	0016506	000206	0015339	20005940
POC	1	1	1	
Data For Record?	Yes	Yes	Yes	No
Purpose				
Objective				
Scale				
Height Above Ground	4.0	4.0	4.0	4.0
Height Above Platform	1.0	1.0	1.0	1.5
Sampler Spacing				
Current Manual Available?	Yes	Yes	Yes	Yes
Instrument Log Up-to-date?	Yes	Yes	Yes	Yes
In-line Filter Change Date	2006-08-02	2006-08-02	2006-08-02	
Cal. Gas Cert. Date	2002-11-05	2002-11-05		
Calibration Current?	Yes	Yes	Yes	Yes
Calibration Date	2006-01-10	2006-01-10	2006-04-18	Not Available
Cal. Equipment Cert. Date	Not Available	Not Available	Not Available	Not Available
Obstacle Description	None	None	None	None
Distance to Obstacle	-	-	-	-
Height Above Inlet	-	-	-	-
Distance to Walls, etc.	-	-	-	-
Distance to Dripline	-	-	-	-
Dominant Influence	Vehicular	Vehicular	Vehicular	Residential
Residence Time (sec)	8.2	8.3	10.5	

## Site Survey Report (Cont.)

Monitor Type	BAM-PM2.5
Manufacturer/Model	Met One BAM1020
Serial Number	A2549
POC	
Data For Record?	No
Purpose	
Objective	
Scale	
Height Above Ground	2.5
Height Above Platform	
Sampler Spacing	
Current Manual Available?	Yes
Instrument Log Up-to-date?	Yes
In-line Filter Change Date	
Cal. Gas Cert. Date	
Calibration Current?	No
Calibration Date	Not Available
Cal. Equipment Cert. Date	Not Available
Obstacle Description	None
Distance to Obstacle	-
Height Above Inlet	-
Distance to Walls, etc.	-
Distance to Dripline	-
Dominant Influence	Vehicular
Residence Time (sec)	