



Quality Assurance Site Information for La Habra

This page updated February 10, 2005

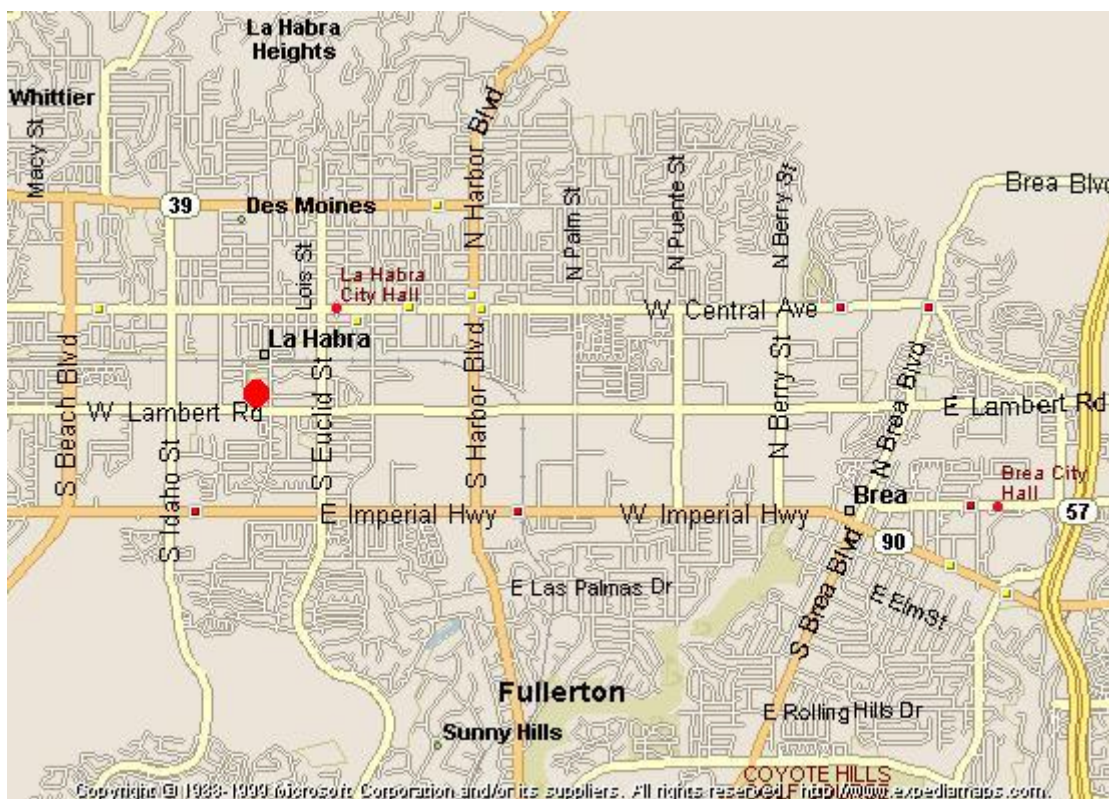

AIRS Number	ARB Number	Site Start Date	Reporting Agency and Agency Code
060595001	30177	1/1/67	South Coast AQMD (061)

Site Address	County	Air Basin	Latitude	Longitude	Elevation
621 W. Lambert, La Habra CA 90631	Orange	South Coast	33° 55' 31"	117° 57' 8"	82

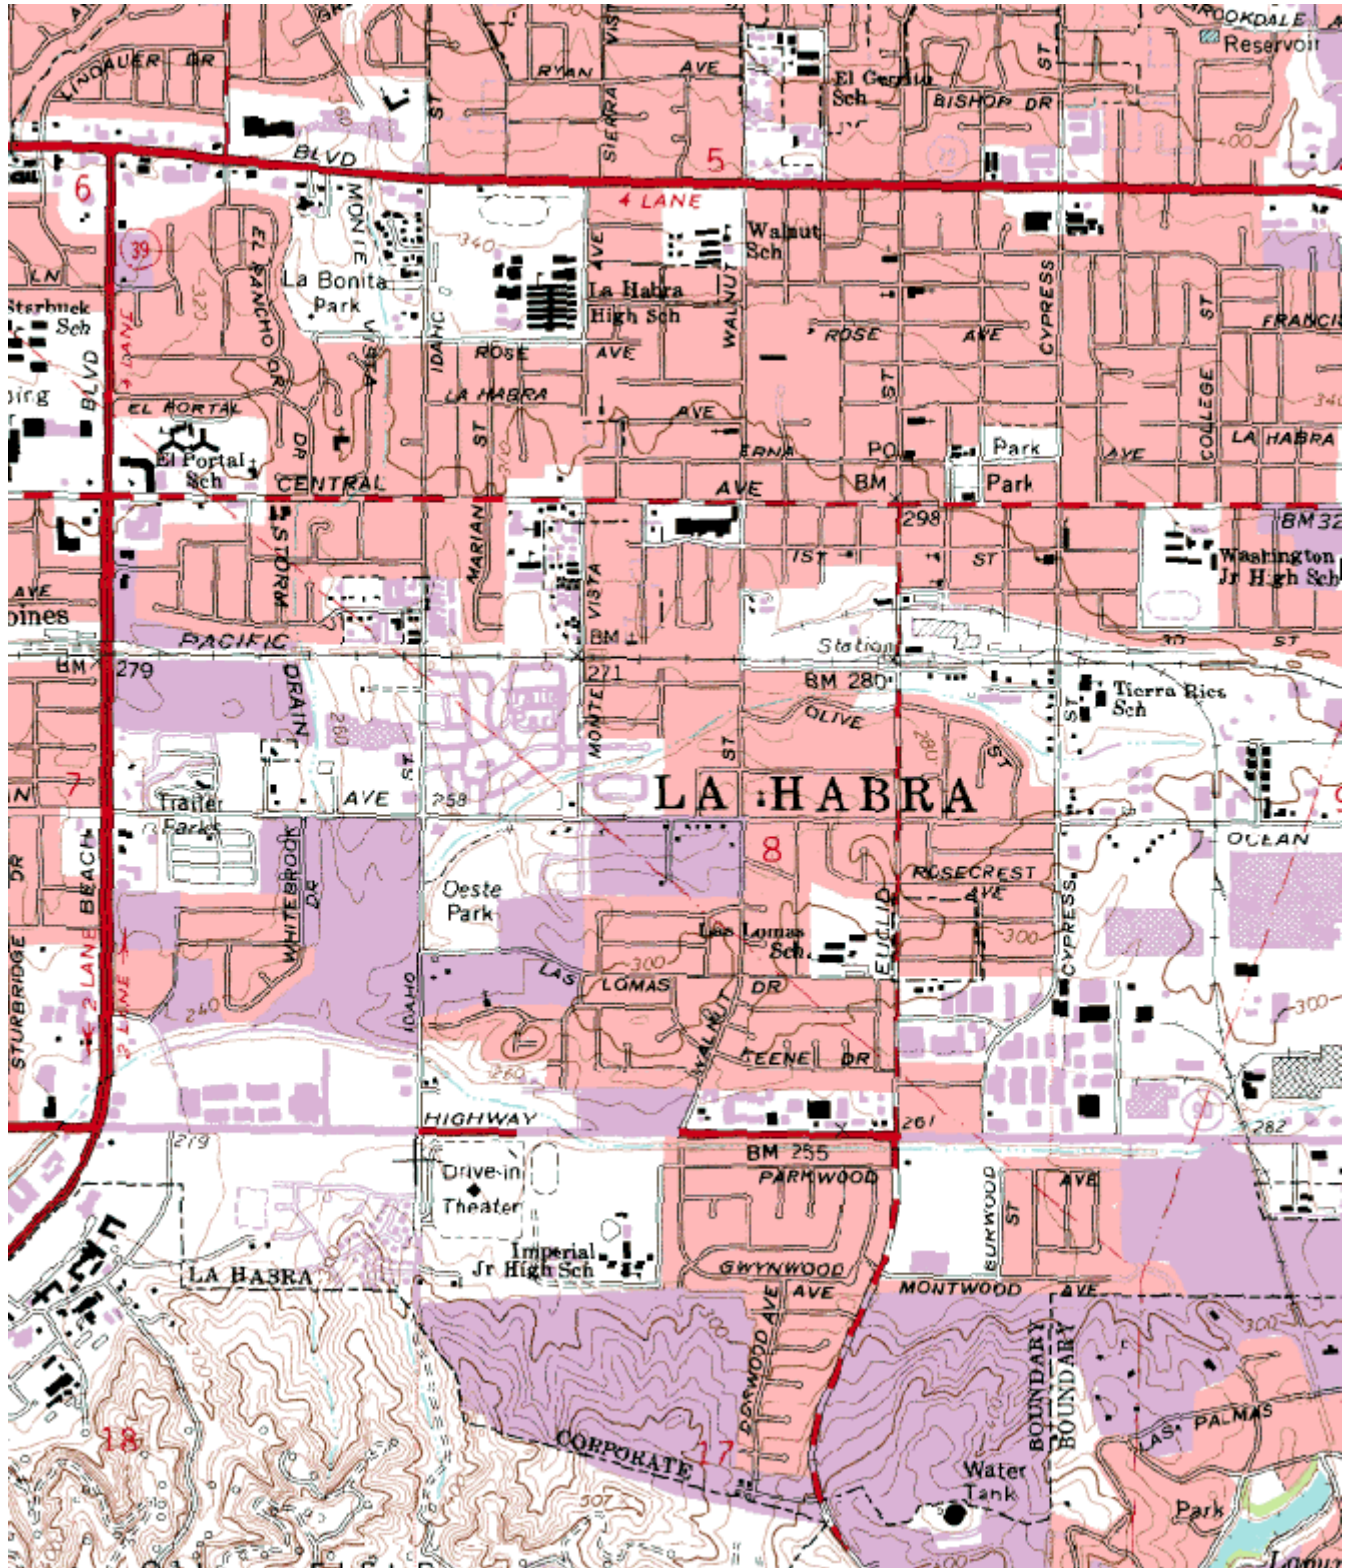

Site Survey Report

Siting Information

Site Name: La Habra	Audit Date: 2005-08-30	ARB Number: 30177	AIRS Number: 060595001
Address: 621 W. Lambert La Habra, CA 90631	Latitude: 33° 55' 31"	Longitude: 117° 57' 8"	Elevation (m): 82
	Auditors: Long Liu Alvin Danque	Site Technician: Charlie Decker	Site Phone:
Operating Agency: South Coast AQMD		Site Report: Yes	Site Photos: Yes

General Siting Conditions

Station Temperature Controlled: Yes Recorded: Yes Inside Temp: 25 Degrees Celsius	Traffic Description: Residential Distance: 100 meters Count (Veh/Day): 1000	Topography Site: Level Region: Level	Predominant Wind Direction: Southwest
			Arc Air Flow (Deg): 360 Degrees
		Meteorology Located With Instruments: Yes Shadowing: No Boom Orientation (Deg): N/A Temp(Motor/Natural): Natural	Non-vehicular Local Sources Description: NA Distance: 0 meters Direction:
Agency: South Coast AQMD Urbanization: City Center Ground Cover: asphalt	Manifold Clean: Yes		
	Cleaning Schedule: As needed		
	Autocalibrator Type: Envirionics 100		
	Site Survey Complete: Yes		
			Logbook Up To Date: Yes

Action Items

Comments

Site Survey Report (Cont.)

Monitor Type	Carbon Monoxide	Nitrogen Dioxide	Ozone
Manufacturer/Model	Horiba APMA-360	API 200	API/Teledyne 400
Serial Number	0016211	e000201	012681
POC	1	2	1
Data For Record?	Yes	Yes	Yes
Purpose			
Objective			
Scale			
Height Above Ground	6.0	6.0	6.0
Height Above Platform	1.5	1.5	1.5
Sampler Spacing			
Current Manual Available?	Yes	Yes	Yes
Instrument Log Up-to-date?	Yes	Yes	Yes
In-line Filter Change Date	2005-08-30	2005-08-30	2005-08-30
Cal. Gas Cert. Date	2004-03-31	2004-03-31	
Calibration Current?	Yes	Yes	Yes
Calibration Date	2005-06-08	2005-06-07	2005-05-26
Cal. Equipment Cert. Date	2005-05-03	2005-05-03	2005-05-03
Obstacle Description	None	None	None
Distance to Obstacle	-	-	-
Height Above Inlet	-	-	-
Distance to Walls, etc.	-	-	-
Distance to Dripline	-	-	-
Dominant Influence	Vehicular	Vehicular	Vehicular
Residence Time (sec)	23.7	25.6	25.8