


Quality Assurance Site Information for Ontario-Fire Station

This page updated February 10, 2005



AIRS Number	ARB Number	Site Start Date	Reporting Agency and Agency Code
060710025	36025	12/11/98	South Coast AQMD (061)

Site Address	County	Air Basin	Latitude	Longitude	Elevation
1408 Francis St, Ontario CA 91761	San Bernardino	South Coast	34° 02' 23"	117° 37' 25"	288

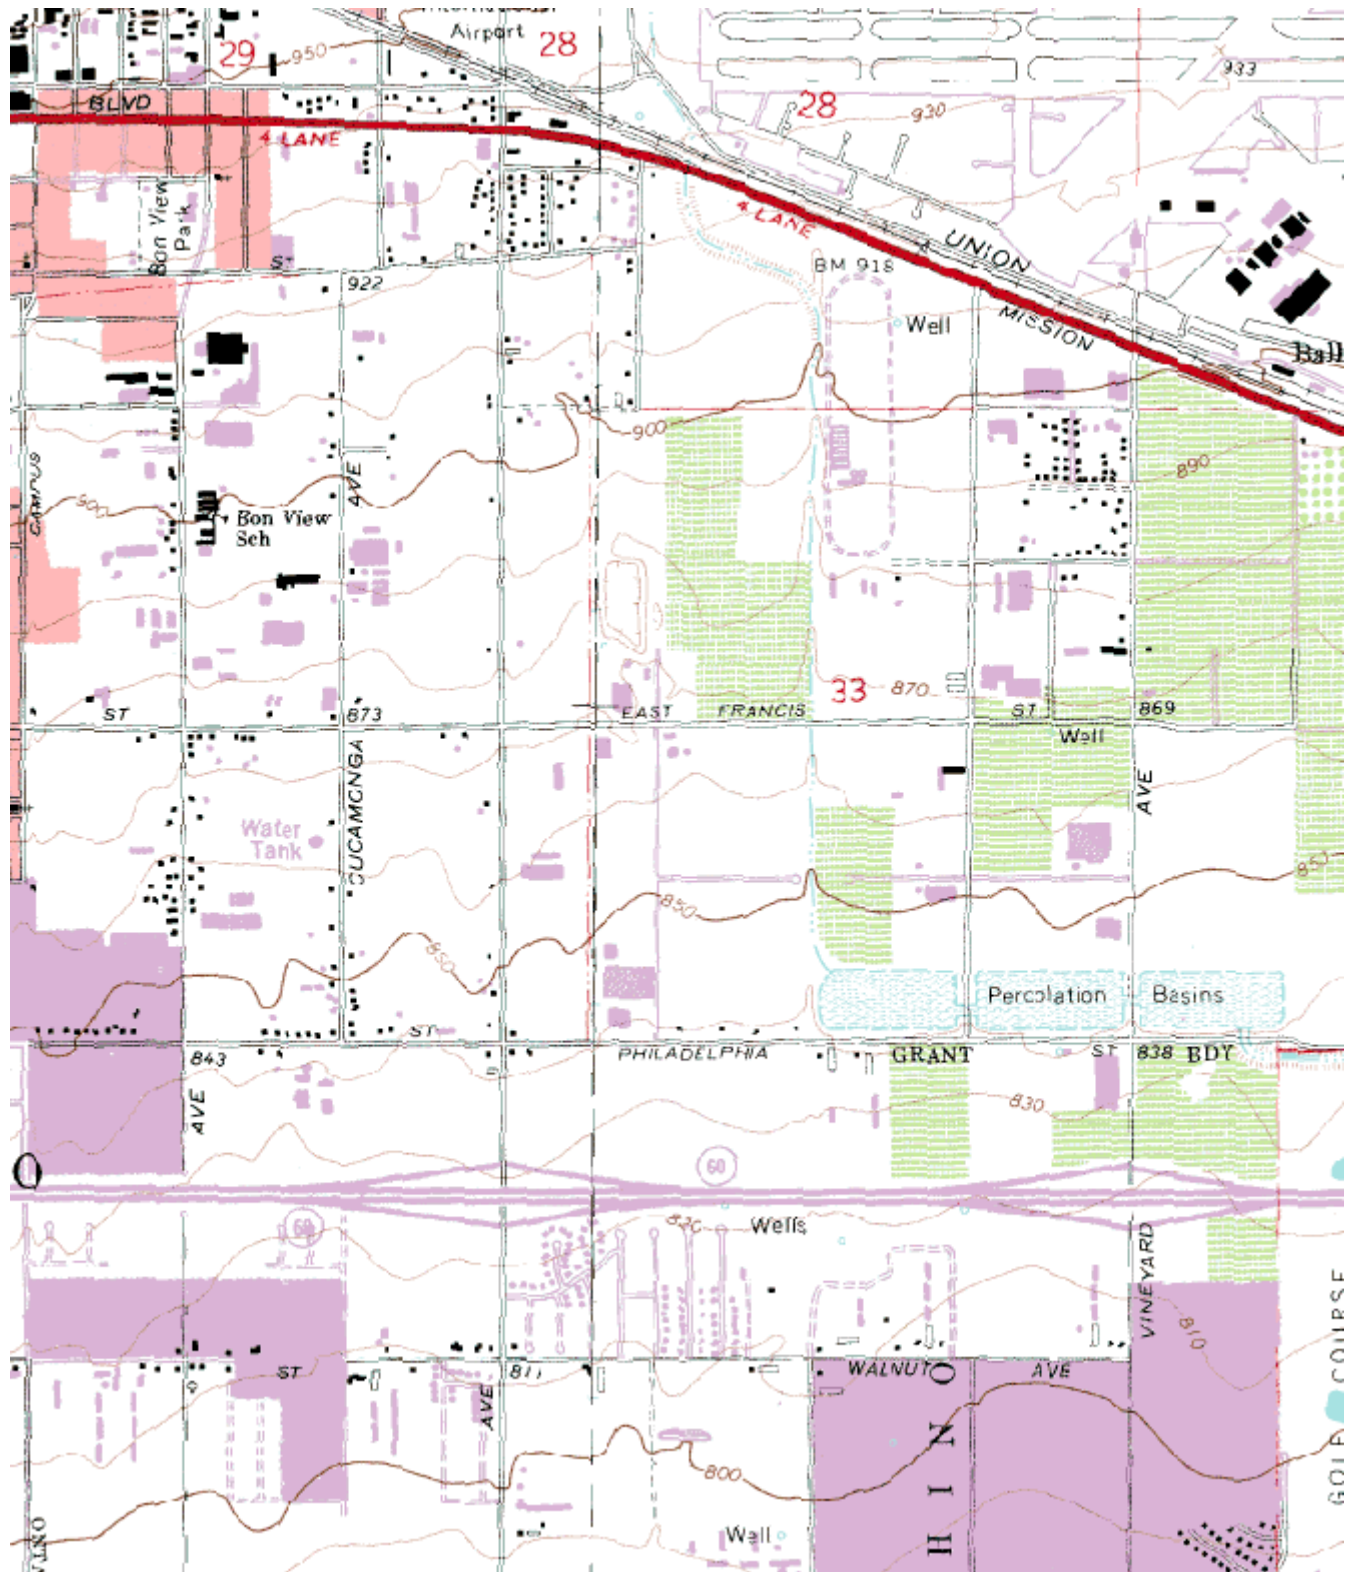

Site Survey Report

Siting Information

Site Name: Ontario-Fire Station	Audit Date: 2006-12-07	ARB Number: 36025	AIRS Number: 060710025
Address: 1408 Francis St Ontario, CA 91761	Latitude: 34° 02' 23"	Longitude: 117° 37' 25"	Elevation (m): 288
	Auditors: Long Liu Dustin Goto	Site Technician: Keith Brown	Site Phone:
Operating Agency: South Coast AQMD		Site Report: Yes	Site Photos: Yes

General Siting Conditions

Station Temperature Controlled: No Recorded: No Inside Temp: 0 Degrees Celsius	Traffic Description: Commercial Distance: 100 meters Count (Veh/Day): 20000	Topography Site: Level Region: Level	Predominant Wind Direction: Northeast
			Arc Air Flow (Deg): 360 Degrees
		Meteorology Located With Instruments: No Shadowing: No Boom Orientation (Deg): N/A Temp(Motor/Natural):	Non-vehicular Local Sources Description: Fire Station Distance: 50 meters Direction: N
Agency: South Coast AQMD	Manifold Clean: N/A		
Urbanization: Suburban	Cleaning Schedule: N/A		
Ground Cover: Gravel	Autocalibrator Type: N/A		
	Site Survey Complete: Yes		
	Logbook Up To Date: Yes		

Action Items

Comments

Site Survey Report (Cont.)

Monitor Type	PM10-SSI	PM10-SSI	PM2.5	PM2.5
Manufacturer/Model	Sierra Anderson 1200	Sierra Anderson 1200	Sierra Anderson RAAS PM2.5	Andersen 300
Serial Number	1532B	4994A	00119	0019
POC	2	1	1	1
Data For Record?	Yes	Yes	Yes	Yes
Purpose				
Objective				
Scale				
Height Above Ground	4.0	4.0	2.9	2.9
Height Above Platform	1.9	1.9	1.9	1.9
Sampler Spacing	6.0	6.0		
Current Manual Available?	Yes	Yes	Yes	Yes
Instrument Log Up-to-date?	Yes	Yes	Yes	Yes
In-line Filter Change Date				
Cal. Gas Cert. Date				
Calibration Current?	Yes	Yes	Yes	Yes
Calibration Date	2006-07-10	2006-07-11	2006-11-03	2006-09-13
Cal. Equipment Cert. Date	Not Available	Not Available	Not Available	Not Available
Obstacle Description	None	None	None	None
Distance to Obstacle	-	-	-	-
Height Above Inlet	-	-	-	-
Distance to Walls, etc.	-	-	-	-
Distance to Dripline	-	-	-	-
Dominant Influence	Vehicular	Vehicular	Vehicular	Vehicular
Residence Time (sec)				