


Quality Assurance Site Information for Perris

This page updated February 10, 2005



AIRS Number	ARB Number	Site Start Date	Reporting Agency and Agency Code
060656001	33149	5/1/73	South Coast AQMD (061)

Site Address	County	Air Basin	Latitude	Longitude	Elevation
237 1/2 N. D St., Perris CA 92570	Riverside	South Coast	33° 47' 20"	117° 13' 40"	442

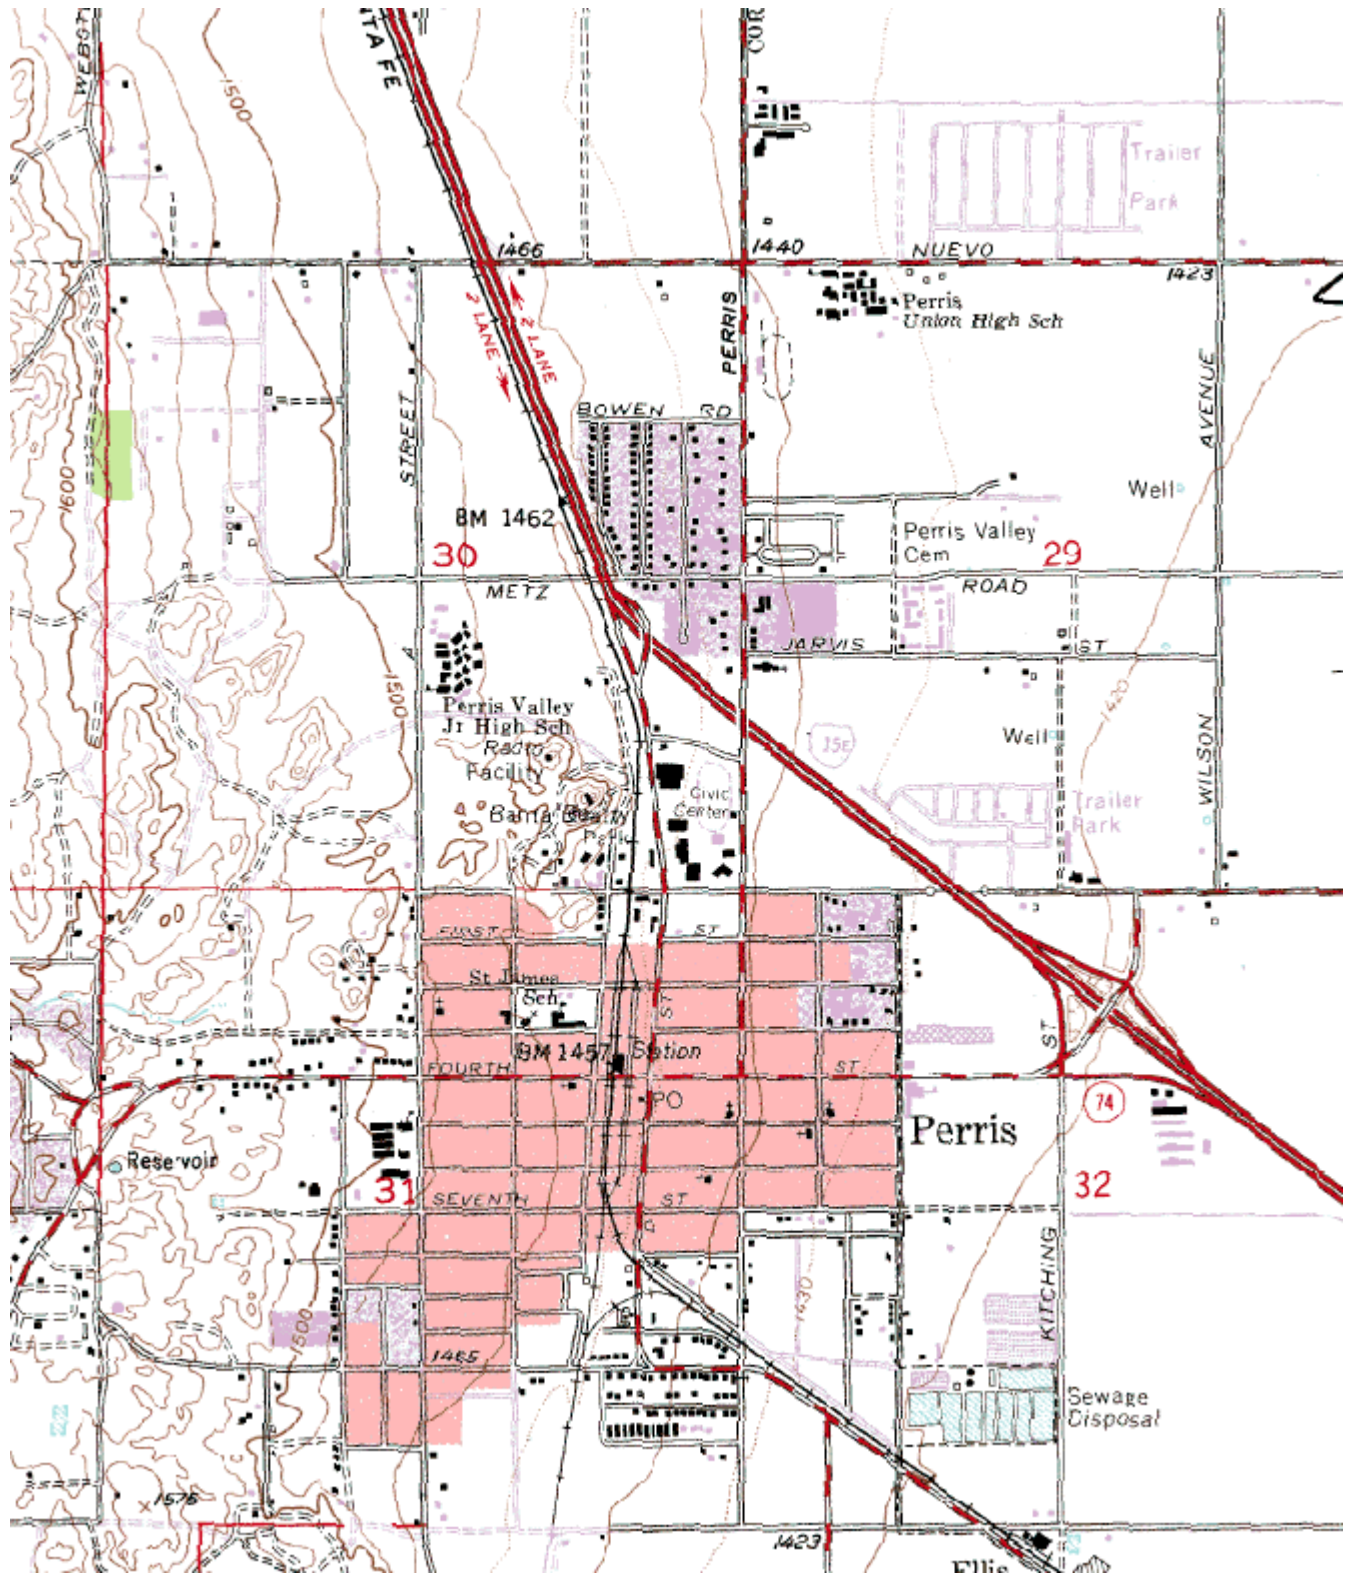

Site Survey Report

Siting Information

Site Name: Perris	Audit Date: 2005-08-29	ARB Number: 33149	AIRS Number: 060656001
Address: 237 1/2 N. D St. Perris, CA 92570	Latitude: 33° 47' 20"	Longitude: 117° 13' 40"	Elevation (m): 442
	Auditors: Alvin Danque Long Liu	Site Technician: Twyla Miner	Site Phone:
Operating Agency: South Coast AQMD		Site Report: Yes	Site Photos: Yes

General Siting Conditions

Station Temperature Controlled: Yes Recorded: Yes Inside Temp: 25 Degrees Celsius	Traffic Description: Arterial Distance: 500 meters Count (Veh/Day): 3000	Topography Site: level Region: level	Predominant Wind Direction: Southeast
			Arc Air Flow (Deg): 360 Degrees
		Meteorology Located With Instruments: Yes Shadowing: No Boom Orientation (Deg): N/A Temp(Motor/Natural): Natural	Non-vehicular Local Sources Description: Distance: 0 meters Direction:
Urbanization: Suburban Ground Cover: asphalt	Manifold Clean: Yes		
	Cleaning Schedule: As needed		
	Autocalibrator Type: Sabio		
Site Survey Complete: Yes			
Logbook Up To Date: Yes			

Action Items

Comments

Site Survey Report (Cont.)

Monitor Type	Ozone	PM10-SSI
Manufacturer/Model	API/Teledyne 400	Sierra Anderson 1200
Serial Number	012722	3980
POC	1	1
Data For Record?	Yes	Yes
Purpose		
Objective		
Scale		
Height Above Ground	3.0	2.0
Height Above Platform	0.5	1.5
Sampler Spacing		
Current Manual Available?	Yes	Yes
Instrument Log Up-to-date?	Yes	Yes
In-line Filter Change Date	Not Available	
Cal. Gas Cert. Date		
Calibration Current?	Yes	Yes
Calibration Date	2005-05-03	2005-08-06
Cal. Equipment Cert. Date	2005-05-03	2004-12-07
Obstacle Description	None	None
Distance to Obstacle	-	-
Height Above Inlet	-	-
Distance to Walls, etc.	-	-
Distance to Dripline	-	-
Dominant Influence	Vehicular	Vehicular
Residence Time (sec)	80.7	