

Improvements in the Blackbody Calibration of Pyrgometers

Ibrahim Reda¹ Julian Gröbner² Tom Stoffel¹ Daryl Myers¹ Bruce Forgan³

1. National Renewable Energy Laboratory (NREL) 2. Physikalisch-Meteorologisches Observatorium Davos, World Radiation Center (PMOD/WRC) 3. Bureau of Meteorology, Australia



Abstract

Pyrgometers are used to measure the atmospheric longwave irradiance through out the ARM program sites. Previous calibrations of pyrgometers using ARM/Eppley/NREL blackbody were consistent, but introduced a difference in the historical clear sky measured irradiance. This difference was believed to be in the order of 12 W/m². In this poster we show the improvements to the blackbody and calibration methodology by comparing our results to the results of a group of pyrgometers that were recently calibrated against the World Infrared Standard Group, in the World Radiation Center, Davos/Switzerland.

Improvements in the Blackbody

- Lower viscosity oil in Blackbody (BB); temperature gradient reduced from 3°C to 0.8°C @ -30°C temperature plateau; clear sky bias reduced from 12 W/m² to 6 W/m²
- Added Wolfgang's thermal mass to increase BB thermal capacity; outdoor data scatter reduced from ± 6 W/m² to ± 2 W/m²
- Proper polishing and gold plating for BB completion hemisphere. Nickel layer inserted between copper and gold to prevent copper/gold diffusion (*Chang, C., 1986, J. Appl.Phys., Vol. 60, No. 3, 1*); improved BB emissivity
- Attached thermistor to gold completion hemisphere, added its emitted irradiance to BB irradiance, $e_6 = 0.02$ (NIST Data); BB irradiance increased by 4 W/m² (± 1 W/m² vs T-plateaus).

Pyrgometer Blackbody Calibration System Simplified Diagram

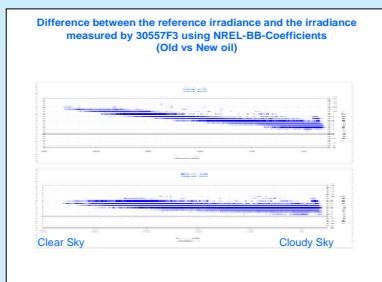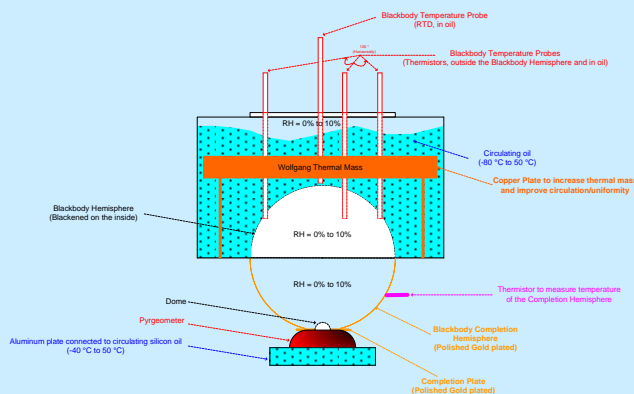

Evaluation Method

- Five pyrgometers calibrated at PMOD, established NREL Reference Group (NRG): 3-PIRs and 2-CG4s
- Calibrated NRG using PMOD Blackbody (BB)
- NRG deployed outdoors at PMOD vs World Infrared Standard Group (WISG) > 4 months
- Adjusted PMOD-BB coefficient (C) to match the WISG irradiance
- Calibrated NRG using NREL Blackbody (BB)
- Using the same outdoor data at Davos, adjusted NREL-BB coefficients (K₁ and K₂) to match the WISG irradiance, and K₃ to reduce scatter
- Compared the results from PMOD's and NREL's BB and outdoor calibrations


PMOD and NREL BB calibration coefficients vs adjusted coefficients to match the WISG irradiance, using PMOD equation												
Coefficient	Source	CG4-19847	CG4-09881	PIR-30557F3	PIR-31197F2	PIR-31237F3	PMOD-BB	NREL-BB	PMOD-BB	NREL-BB	PMOD-BB	NREL-BB
C	BB	11.952	0.543	1.665	0.222	0.228	4.158	3.473	3.473	3.473	3.473	3.473
	Adjusted	12.261	11.565	0.366	1.965	0.475	3.655	4.223	3.655	3.655	3.655	3.220
K1	BB	0.22111	0.27120	0.22671	0.22623	0.22623	0.22623	0.22623	0.22623	0.22623	0.22623	0.22623
	Adjusted	0.22675	0.22647	0.22675	0.22675	0.22675	0.22675	0.22675	0.22675	0.22675	0.22675	0.22675
K2	BB	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.01
	Adjusted	0.00995	0.00995	0.00995	0.00995	0.00995	0.00995	0.00995	0.00995	0.00995	0.00995	0.00995
K3	BB	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.01
	Adjusted	0.00995	0.00995	0.00995	0.00995	0.00995	0.00995	0.00995	0.00995	0.00995	0.00995	0.00995
RMSE (W/m²)		1.3	1.3	1.1	1.9	2.2	1.2	1.2	1.2	1.2	1.2	1.2

PMOD and NREL BB calibration coefficients vs adjusted coefficients to match the WISG irradiance, using NREL equation												
Coefficient	Source	CG4-19847	CG4-09881	PIR-30557F3	PIR-31197F2	PIR-31237F3	PMOD-BB	NREL-BB	PMOD-BB	NREL-BB	PMOD-BB	NREL-BB
W0	BB	2.26	-11.2	0.599	-0.36	-1.77	-11.81	0.46	-11.2	0.172	-17.53	-17.53
	Adjusted	0.269	0.269	0.116	0.116	0.2174	0.223	0.223	0.223	0.223	0.223	0.223
K1	BB	0.2175	0.2175	0.2175	0.2175	0.2175	0.2175	0.2175	0.2175	0.2175	0.2175	0.2175
	Adjusted	0.2175	0.2175	0.2175	0.2175	0.2175	0.2175	0.2175	0.2175	0.2175	0.2175	0.2175
K2	BB	0.2998	0.2998	0.2998	0.2998	0.2998	0.2998	0.2998	0.2998	0.2998	0.2998	0.2998
	Adjusted	1.03	1.03	1.03	1.03	1.03	1.03	1.03	1.03	1.03	1.03	1.03
K3	BB	NA	NA	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.01
	Adjusted	NA	NA	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.01
RMSE (W/m²)		1.3	1.3	1.1	1.9	2.2	1.2	1.2	1.2	1.2	1.2	1.2

Comments/Conclusions

1. NREL-BB improvements reduced ~12 W/m² bias to (-1 to 3) W/m² w.r.t. WISG
2. What is the absolute value?
Can it be FROM:
- IPASRC-I; Present WISG?
- IPASRC-II; 2.5 W/m² to 3 W/m² lower than IPASRC-I?
- Outdoor calibration independent from reference irradiance (*Reda et al., 2006, J. Atmospheric and Solar Terrestrial Physics, 68, 1416-1424*); ± 3 W/m² from WISG?
- Improved NREL-BB; -1 W/m² to 3 W/m² from WISG?
3. The BB calibration coefficients must be adjusted outdoors to an Internationally accepted reference (i.e. WISG) for global uniformity, and to account for the spectral response of pyrgometers and the mismatch between the BB (indoors) and the outdoors
4. Other pyrgometer calibration systems are needed to evaluate the WISG to establish a consensus reference with traceability to SI units.

Applying Results of Both International Pyrgometer and Absolute Sky-scanning Radiometer Comparisons (IPASRC)

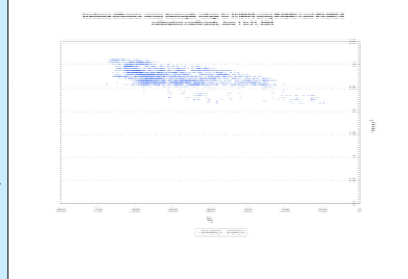

$$\text{PMOD Equation: } W_0 = \frac{V}{C} \cdot (1 + k_1 \cdot \sigma + k_2 \cdot W_0 - k_3 \cdot (W_0 - W_1)) \quad \text{NREL Equation: } W_0 = K_0 + K_1 \cdot V + K_2 \cdot W_0 - K_3 \cdot (W_0 - W_1)$$

