

---

**Method 1648**

**Organic Halides in Solid Matrices by Neutron Activation Analysis**

---

**June 1991**

**U.S. Environmental Protection Agency  
Office of Science and Technology  
Engineering and Analysis Division  
401 M Street S.W.  
Washington, D.C. 20460**

---

## Method 1648

### Organic Halides in Solid Matrices by Neutron Activation Analysis

#### 1.0 Scope and Application

- 1.1 This method is designed to meet the survey requirements of the United States Environmental Protection Agency (EPA). It is used to determine organic halides associated with the Clean Water Act; the resources Conservation and Recovery Act; the Comprehensive Environmental Response, Compensation and Liability Act; and other organic halides amenable to adsorption and Neutron Activation Analysis.
- 1.2 The method is applicable to the determination of organic halides in soils, sludges, and pulp. The method is a combination of existing methods and new technology for organic halide measurement.
- 1.3 This method is for use by or under the supervision of analysts experienced in the use of Neutron Activation. Each laboratory that uses this method must demonstrate the ability to generate acceptable results using the procedure in Section 8.2.
- 1.4 Any modification of this method beyond those expressly permitted is subject to the application and approval of alternate test procedures under 40 CFR Parts 134 and 135.

#### 2.0 Summary of Method

- 2.1 Sample Preparation—Organic halides are leached from the sample into water by acidification and sonication. The organic halides in the leachate are adsorbed onto granular activated carbon (GAC). The sample and GAC are collected on a polycarbonate filter.
- 2.2 Sample Analysis—Neutron Activation Analysis (NAA) the sample, GAC, and filter are placed in a vial and sealed. The vial is exposed to radiation. Unique radioisotopes of Cl are produced. These are measured using a gamma-ray detector to determine the total Cl.
- 2.3 The mass concentration of organic halides is reported as an equivalent concentration of organically bound chloride (Cl).

#### 3.0 Contamination and Interferences

- 3.1 Solvents, reagents, glassware, and other sample processing hardware may yield elevated readings from the microcoulometer. All materials used in the analysis shall be demonstrated to be free from interferences under the conditions of analysis by running method blanks initially and with each sample set (samples started through the adsorption process in a given 8 hour shift, to a maximum of 20). Specific selection of reagents and purification of solvents may be required.
- 3.2 Glassware is cleaned by detergent washing in hot water, rinsing with tap water and distilled water, capping with aluminum foil, and baking at 450°C for one hour minimum. For some glassware, immersion in chromate cleaning solution prior to

detergent washing may be required. If blanks from glassware without cleaning or with fewer cleaning steps show no detectable organic halide, the cleaning steps that do not eliminate organic halide may be omitted.

3.3 The most common contamination results from methylene chloride vapors in laboratories that perform organic extractions. Heating, ventilating, and air conditioning systems that are shared between the extraction laboratory and the laboratory in which organic halide measurements are performed transfer the methylene chloride vapors to the air in the organic halide laboratory. Exposure of the activated carbon used in the analysis results in contamination. Separate air handling systems, charcoal filters, and glove boxes can be used to minimize this exposure.

### 3.4 Activated Carbon

3.4.1 Purity of each lot of activated carbon must be verified before each use measuring the adsorption capacity and the background level of halogen (Section 8.5). The stock of activated carbon should be stored in its granular form in a glass container that is capped tightly. Protect carbon at all times from all sources of halogen vapors.

3.4.2 Inorganic substances such as chloride, chlorite, bromide, and iodide will adsorb on activated carbon to an extent dependent on their original concentration in the aqueous solution and the volume of sample adsorbed. Treating the activated carbon with a solution of nitrate causes competitive desorption of inorganic halide species. However, if the inorganic halide concentration is greater than 2,000 times the organic halide concentration, artificially high results may be obtained.

3.4.3 Halogenated organic compounds that are weakly adsorbed on activated carbon are only partially recovered from the sample. These include certain alcohols and acids such as chloroethanol and chloroacetic acid that can be removed from activated carbon by nitrate wash.

3.5 Polyethylene gloves should be worn when handling equipment surfaces in contact with the sample.

## 4.0 Safety

4.1 The toxicity or carcinogenicity of each reagent used in this method has not been precisely determined; however, each chemical substance should be reduced to the lowest possible level. The laboratory is responsible for maintaining a current awareness file of OSHA regulations regarding the safe handling of the chemicals specified in this method. A reference file of material safety data sheets should be available to all personnel involved in the chemical analysis. Additional information on laboratory safety can be found in References 9-11.

4.2 This method employs strong acids. Appropriate clothing, gloves, and eye protection should be worn when handling these substances.

- 4.3 Field samples may contain high concentrations of toxic volatile compounds. Sample containers should be opened in a hood and handled with gloves that will prevent exposure.

## 5.0 Apparatus and Materials

### 5.1 Sampling Equipment

5.1.1 Four ounce glass jar—Chromic acid rinse, detergent water wash, rinse with tap and distilled water, cover with aluminum foil and heat to 450°C for one hour minimum before use.

5.1.2 Teflon liner—Cleaned as above and baked at 100-200°C for one hour minimum.

5.1.3 Jars and liners must be lot certified to be free of organic halides by running blanks according to this method.

- 5.2 Scoop of Granular Activated Carbon (GAC)—capable of precisely measuring 0.13 ±0.01 cc GAC (Dohrmann Measuring Cup 521-021, or equivalent). This scoop size has been shown to hold 35-60 mg of GAC, depending on the source.

### 5.3 Adsorption Apparatus

5.3.1 Finger type sonicator capable of developing 100-110 watts at 50% duty-Cycle. (Branon Model 450 or equivalent)

5.3.2 20 mL vials used for sample sonication.

5.3.3 Adsorption System—Rotary shaker, wrist action shaker, or other system for assuring thorough contact of sample with activated carbon. The system used shall be demonstrated to meet the performance requirements in Section 8 of this method.

5.3.3.1 Erlenmeyer flasks—250 mL with ground glass stopper, for use with rotary shaker.

5.3.3.2 Shake table—Sybron Thermolyne Model LE "Big Bill" rotator/shaker, or equivalent.

5.3.3.3 Rack attached to shake table to permit agitation of 16-25 samples simultaneously.

5.3.4 Filtration system—Figure 1

5.3.4.1 Vacuum filter holder—Glass, with fritted glass support (Fisher Model 09-753E, or equivalent).

5.3.4.2 Polycarbonate filter—0.45 micron, 25 mm diameter, (Micro Separation Inc, Model K04CP02500, or equivalent).

- 5.3.4.3 Filter forceps—Fisher Model 09-753-50, or equivalent, for handling filters. Clean by washing with detergent and water, rinsing with tap and deionized water, and air drying on aluminum foil. Two forceps may better aid in handling filters. Clean by washing with detergent and water, rinsing with tap and deionized water, and air drying on aluminum foil.
- 5.3.4.4 Vacuum flask—500 mL (Fisher 10-1800, or equivalent).
- 5.3.4.5 Vacuum Source—A pressure/vacuum pump, rotary vacuum pump, or other vacuum source capable of providing at least 610 mm (24 in) Hg vacuum and 30 L/min free air displacement.
- 5.3.4.6 Stopper and tubing to mate the filter holder to the flask and the flask to the pump.
- 5.3.4.7 Polyethylene gloves—for handling filters (Fisher 11-394-110-B, or equivalent).

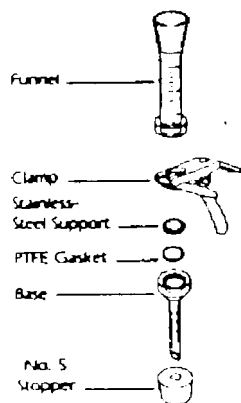


Figure 1 Filter Apparatus

## 5.5 Neutron Activation System

- 5.5.1 Containers suitable for containment of samples and standards during irradiation (e.g., 1/5-dram polyethylene snap-cap vial).
- 5.5.2 Sample introduction system and a reactor generating a thermal neutron flux capable of achieving enough halogen activity for counting purposes (e.g., reactor having a neutron flux of  $5 \times 10^{12}$  neutrons/cm<sup>2</sup>/sec).
- 5.5.3 Lithium-drifted germanium [Ge(Li)] gamma-ray detector with an amplifier and a 4096-channel memory unit for data storage system capable of resolving the halogen peaks from potential interferences and background.

## 5.6 Miscellaneous Glassware

- 5.6.1 Volumetric flasks—5, 10, 25, 50, 100, and 1000 mL.
- 5.6.2 Beakers—100, 500, and 1000 mL.
- 5.6.3 Volumetric pipets—1 and 10 mL with pipet bulbs.
- 5.6.4 Volumetric micro-pipets—10, 20, 50, 100, 200, and 500  $\mu\text{L}$  with pipet control (Hamilton 0010, or equivalent).
- 5.6.5 Graduated cylinders—10, 100, and 1000 mL.

## 5.7 Micro-Syringes—10, 50, and 100 $\mu\text{L}$ .

## 5.8 Balances

- 5.8.1 Top loading—Capable of weighing 0.1 g.
- 5.8.2 Analytical—Capable of weighing 0.1 mg.

## 5.9 Wash Bottles—500-1000 mL, Teflon or polyethylene.

## 6.0 Reagents and Standards

6.1 Granular Activated Carbon (GAC)—75-150  $\mu\text{m}$  (100-200 mesh), (Dorhmann 511-877, or equivalent), with chlorine content less than 1  $\mu\text{g Cl}^-$  per scoop (<25  $\mu\text{g Cl}$  per gram), adsorption capacity greater than 1000  $\mu\text{g Cl}^-$  (2,4,6-trichlorophenol) per scoop (>10,000  $\mu\text{g}$  per gram), inorganic halide retention of less than 1  $\mu\text{g Cl}^-$  per scoop in the presence of 2500 mg of inorganic halide), and that meets the other test criteria in Section 8.5 of this method.

6.2 Reagent Water—Water in which organic halide is not detected by this method.

6.2.1 Preparation—Reagent water may be generated by:

6.2.1.1 Activated carbon—Pass tap water through a carbon bed (Calgon Filtrasorb-300, or equivalent).

6.2.1.2 Water purifier—Pass tap water through a purifier (Millipore Super Q, or equivalent).

6.2.2 pH adjustment—Adjust the pH of the reagent water to <2 with nitric acid for all reagent water used in this method.

6.3 Nitric Acid ( $\text{HNO}_3$ )—Concentrated, analytical grade.

6.4 Nitrate Stock Solution—In a 1000 mL volumetric flask, dissolve 17 g of  $\text{NaNO}_3$  in approx 100 mL of water, add 1.4 mL nitric acid (Section 6.3) and dilute to the mark with reagent water.

- 6.5 Nitrate Wash Solution—Dilute 50 mL of nitrate stock solution (Section 6.4) to 1000 mL with reagent water.
- 6.6 Sodium Thiosulfate ( $\text{Na}_2\text{S}_2\text{O}_3$ ) Solution (1 N)—Weigh 79 g  $\text{Na}_2\text{S}_2\text{O}_3$  in a 1 L volumetric flask and dilute to the mark with reagent water.
- 6.7 Trichlorophenol Solutions
  - 6.7.1 Trichlorophenol stock solutions (1.0 mg/mL of Cl)—Dissolve 0.186 g of 2,4,6-trichlorophenol in 100 mL of halide-free methanol.
  - 6.7.2 Trichlorophenol precision and recovery standard—Place 50 mg of quartz sand in a 20 mL vial and add 100  $\mu\text{L}$  of trichlorophenol stock solution (Section 6.7.1).
- 6.8 Irradiation Standard
  - 6.8.1 Sodium chloride (NaCl) solution (100  $\mu\text{g}/\text{mL}$  of Cl)—Dissolve 0.165 g NaCl in 1000 mL of reagent water.
  - 6.8.2 Place 250  $\mu\text{L}$  of sodium chloride solution (Section 6.8.1) and 1 mL of reagent water in an irradiation container. Seal container according to Section 10.16.1.

## 7.0 Calibration

- 7.1 Calibration for the Gamma Ray Detector
  - 7.1.1 The gamma ray detector must be calibrated. At the beginning of each eight hour shift prior to making any determinations for this method.
  - 7.1.2 Using a radioactive standard such as cobalt-60 or radium-226, determine the energy of the gamma-ray emitted.
  - 7.1.3 Adjust the gamma-ray detector to fall within one channel ( $\pm 0.5$  KeV) of the radioactive standard's true energy.
  - 7.1.4 Count a 100 second blank to verify that no stray radioactive sources are within sensing distance of the detector.
- 7.2 Calibration for Neutron Activation System—Calibration for entire OX system is performed when the system is set up and when calibration cannot be verified (Section 11).
  - 7.2.1 Background level of Cl—Determine the average background level of Cl for the entire analytical system as follows:
    - 7.2.1.1 Using the procedure in Section 10 that will be used for the analysis of samples, determine the background level of Cl in each of three 50 mg portions of quartz sand.

- 7.2.1.2 Calculate the average (mean) concentration of  $\text{Cl}^-$  and the standard deviation of the concentration.
- 7.2.1.3 The sum of the average concentration plus two times the standard deviation of the concentration shall be less than  $2 \mu\text{g}$  of  $\text{Cl}^-$ . If not, the water or carbon shall be replaced, or the adsorption system moved to an area free of organic halide vapors, and the test (Section 7.5) shall be repeated. Only after this is passed may calibration proceed.
- 7.2.2 Calibration by external standard—A calibration curve encompassing the calibration range is performed using 2,4,6-trichlorophenol.
- 7.2.2.1 Place 50 mg of quartz sand in each of five 20 mL vials.
- 7.2.2.2 Pipet 20, 50, 100, 300, and 800  $\mu\text{L}$  of trichlorophenol stock solution (Section 6.7.1) into the vials from Section 7.2.2.1.
- 7.2.2.3 Proceed with the analysis of each sample as per Section 10.
- 7.2.2.4 Using the calculations in Section 12.1 determine the halide present in standard vial.
- 7.2.2.5 Subtract the average value of the background (Section 7.5.2) from each of the five determinations.
- 7.2.2.6 Calibration factor (ratio of response to concentration)—Using the blank subtracted results, compute the calibration factor at each calibration point, and compute the average calibration factor and the relative standard deviation (coefficient of variation;  $C_v$ ) of the calibration factor over the calibration range.
- 7.2.2.7 Linearity—The  $C_v$  of the calibration factor shall be less than 20%; otherwise, the calibration shall be repeated after system corrections have been made.

## 8.0 Quality Assurance/Quality Control

- 8.1 Each laboratory that uses this method is required to operate a formal quality assurance program. The minimum requirements of this program consist of an initial demonstration of laboratory capability, an ongoing analysis of standards and blanks as tests of continued performance, and analysis of matrix spike and matrix spike duplicate (MS/MSD) samples to assess accuracy and precision. Laboratory performance is compared to establish performance criteria to determine if the results of analyses meet the performance characteristics of the method.
- 8.1.1 The analyst shall make an initial demonstration of the ability to generate acceptable accuracy and precision with this method. This ability is established as described in Section 8.2.



- 8.1.2 The analyst is permitted to modify this method to improve performance or lower the costs of measurements provided all performance specifications are met. Each time a modification is made to the method, the analyst is required to repeat the procedures in Sections 7.2 through 7.5 and Section 8.2 to demonstrate method performance.
- 8.1.3 The laboratory shall spike 10% of samples with known concentrations of 2,4,6-trichlorophenol to monitor method performance and matrix interferences (interferences caused by the sample matrix). This test is described in Section 8.3. When results of these spikes indicate atypical method performance for samples, the samples are diluted to bring method performance within acceptable limits.
- 8.1.4 Analyses of blanks are required to demonstrate freedom from contamination. The procedures and criteria for analysis of a blank are described in Section 8.4.
- 8.1.5 The laboratory shall, on an on-going basis, demonstrate through the analysis of the precision and recovery standard that the analysis system is in control. These procedures are described in Section 11.
- 8.1.6 The laboratory shall perform quality control tests on the granular activated carbon. These procedures are described in Section 8.5
- 8.2 Initial Precision and Recovery (IPR)—To establish the ability to generate acceptable precision and recovery, the analyst shall perform the following operations.
  - 8.2.1 Analyze four PAR standards (Section 6.7.2) according to the procedure in Section 10.
  - 8.2.2 Using the results of the set of four analyses, compute the average percent recovery ( $X$ ) and the standard deviation of the percent recovery ( $s$ ) for the results.
  - 8.2.3 The average percent recovery shall be in the range of 7.7-10.8  $\mu\text{g}$  and the standard deviation shall be less than 0.7  $\mu\text{g}$ . If  $X$  and  $s$  meet these acceptance criteria, system performance is acceptable and analysis of blanks and samples may begin. If, however,  $s$  exceeds the precision limit or  $X$  falls outside the range for recovery, system performance is unacceptable. In this case, correct the problem and repeat the test.
- 8.3 Matrix Spikes—The laboratory shall spike a minimum of 10% of samples from a given matrix type (e.g., soil, sludges, and pulps) in duplicate (MS/MSD). If only one sample from a given matrix type is analyzed, an additional two aliquots of that sample shall be spiked.
  - 8.3.1 The concentration of the analytes spiked into the MS/MSD shall be determined as follows:
    - 8.3.1.1 If, as in compliance monitoring, the concentration of OX is being checked against a regulatory concentration limit, the spiking level shall be at that limit or at one to five times higher than the background

concentration determined in Section 8.3.2, whichever concentration is higher.

8.3.1.2 If the concentration of OX is not being checked against a regulatory limit, the spike shall be at the concentration of the PAR standard (Section 6.7.2) or at one to five times higher than the background concentration determined in Section 8.3.2, whichever concentration is higher.

8.3.2 Analyze one sample out of each set of 10 samples from each matrix to determine the background concentration (B) of OX. Spike two additional sample aliquots with spiking solution and analyze them to determine the concentration after spiking (A).

8.3.2.1 Compute the percent recovery (P) of each analyte in each aliquot:

$$P = 100 (A - B)/T$$

where,

T = The true value of the spike.

8.3.2.2 Compute the relative percent difference (RPD) between the two results (not between the two recoveries):

$$RPD = \frac{|(A1 - A2)|}{1/2 (A1 + A2)} \times 100$$

8.3.2.3 If the RPD is less than 20%, and the recoveries for the MS and MSD are within the range of 75-125%, the results are acceptable.

8.3.2.4 If the RPD is greater than 20%, analyze two aliquots of the PAR standard (PAR).

8.3.2.4.1 If the RPD for the two aliquots of the PAR is greater than 20%, the analytical system is out of control. In this case, repair the problem and repeat the analysis of the sample set, including the MS/MSD.

8.3.2.4.2 If, however, the RPD for the two aliquots of the PAR is less than 20%, the sample chosen for the MS/MSD is diluted by a factor of 10 and the MS/MSD test is repeated. If the RPD is still greater than 20%, the result may not be reported for regulatory compliance purposes. In this case, choose another sample for the MS/MSD and repeat analysis of the sample set.

- 8.3.2.5 If the percent recovery for both the MS and MSD are less than 71% or greater than 116%, analyze the precision and recovery (PAR) standard.
- 8.3.2.5.1 If the recovery of the PAR is outside the 71-116% range, the analytical system is out of control. In this case, repair the problem and repeat the analysis of the sample set, including the MS/MSD.
- 8.3.2.5.2 If the recovery of the PAR is within the range of 71-116%, the sample, MS, and MSD are diluted by a factor of 10 and re-analyzed. If the results of the dilute analyses remain outside of the acceptable range, these results may not be reported for regulatory compliance purposes. In this case, choose another sample for the MS/MSD and repeat the analysis of the sample set.
- 8.4 Blanks—Quartz sand blanks are analyzed to demonstrate freedom from contamination.
- 8.4.1 Analyze a quartz sand blank with each set of samples. The blank must be analyzed immediately following calibration verification to demonstrate freedom from contamination and memory effects and must include all details of the procedure to be followed when analyzing samples.
- 8.4.2 If greater than 2  $\mu\text{g}$  of  $\text{Cl}^-$  is found in the blank, analysis of samples is halted until the source of contamination is eliminated and a blank shows no evidence of contamination at this level.
- 8.5 Granular Activated Carbon (GAC) Testing—Each batch of activated carbon is tested before use to ensure adequate quality. Use only GAC meeting the test criteria below.
- 8.5.1 Contamination test—Analyze a scoop of GAC. Reject carbon if the amount of OX exceeds 1  $\mu\text{g}$  (25  $\mu\text{g}$   $\text{Cl}^-/\text{g}$ ).
- 8.5.2 Inorganic chloride adsorption test—Attempt to adsorb NaCl from 10 mg in reagent water. Wash with nitrate solution and analyze. The amount of halide should be less than 1  $\mu\text{g}$   $\text{Cl}^-$  larger than the blank. A larger amount indicates significant uptake of inorganic chloride by the carbon. Reject carbon if the 1  $\mu\text{g}$  level is exceeded.
- 8.5.3 Carbon capacity test—Prepare an adsorption test standard solution in reagent water to contain 10 mg/L organic carbon (as humic acids of equivalent) and an organic halide concentration of 100  $\mu\text{g}/\text{L}$  organo-chloride (from 2,4,6-trichlorophenol). Prepare a blank solution containing only the 10 mg organic carbon. Analyze 100 mL portions of these solutions. Subtract the result of the blank from the result of the halide spike, compare the blank subtracted result to the true value of the spike. Recovery of the halide should be greater than 85%.
- 8.6 The specifications contained in this method can be met if the apparatus used is calibrated properly and maintained in a calibrated state. The standards used for

calibration (Section 7), calibration verification (Section 11), and for the initial (Section 8.2) and ongoing (Section 11) precision and recovery should be identical, so that the most precise results will be obtained.

- 8.7 Depending on specific program requirements, field duplicates may be collected to determine the precision of the sampling technique.

## 9.0 Sample Collection and Preservation

- 9.1 Collect sample in a 4 oz. jar. This will provide a sufficient amount of all quality control testing.
- 9.2 Cool and maintain sample temperature at 0-4°C from the time of collection until analysis.
- 9.3 No holding times have been established for this method.

## 10.0 Sample Preparation

- 10.1 Composite small amounts of sample by mixing small amounts of sample in a clean beaker. The composited sample should total about 1 g and should be taken from three to five points within the sample container. Mix the sub sample well with a stainless steel spatula or glass rod to insure homogeneity.
- 10.2 Weigh out three 50 mg aliquots of the composited sample into 20 mL vials.
- 10.3 Add 5 mL of reagent water to each vial.
- 10.4 Place sonication horn inside the vial and sonicate for five minutes.
- 10.5 Quantitatively transfer the contents of each vial into a 250 mL erlenmeyer flask with 95 mL of reagent water.
- 10.6 Add 100  $\mu$ L of 1 M  $\text{Na}_2\text{S}_2\text{O}_3$  to convert all active Cl to inorganic Cl.
- 10.7 Acidify the samples to a pH of <2 with concentrated  $\text{HNO}_3$ , approximately 200  $\mu$ L.
- 10.8 Add 5 mL of the nitrate stock solution.
- 10.9 Add one level scoop of activated carbon.
- 10.10 Shake the suspension for one hour minimum in a mechanical shaker.
- 10.11 Filter the suspension through a polycarbonate membrane filter. Filter by suction until the liquid level reaches the top of the carbon.
- 10.12 Wash the inside surface of the filter funnel with approximately 25 mL of nitrate wash solution in several portions. After the level of the final wash reaches the top of the charcoal, filter by suction until the cake is barely dry. The time required for drying should be minimized to prevent exposure of the GAC to halogen vapors in the air, but should be sufficient to permit drying of the cake so that excess water is not

- introduced into the combustion apparatus. A drying time of approximately 10 seconds under vacuum has been shown to be effective for this operation.
- 10.13 Carefully remove the top of the filter holder, making sure that no carbon is lost. This operation is most successfully performed by removing the clamp, tilting the top of the filter holder (the funnel portion) to one side, and lifting upward.
- 10.14 Using a squeeze bottle or micro syringe, rapidly rinse the carbon from the inside of the filter holder onto the filter cake using small portions of wash solution. Allow the cake to dry under vacuum for no more than 10 seconds after the final rinse. Immediately turn the vacuum off.
- 10.15 Using the tweezers, carefully fold the polycarbonate filter in half, then in fourths, making sure that no carbon is lost.
- 10.16 Halide Determination by NAA
- 10.16.1 Place filter from Section 10.15 in a prewashed plastic container (e.g., 1/5-dram polyethylene snap-cap vial). The vial has been prewashed to remove inorganic and organic chlorine by a soak in distilled water, followed by storage in a glass jar containing 50% v/v acetone and hexane. After cleaning, the vial is removed by forceps and air-dried to remove residual water, acetone, and hexane. After the carbon is placed in the vial, the vial is snapped shut, the hinge removed with a scalpel blade, the cap heat-sealed to the vial with an electric soldering gun reserved for that purpose, and an indentifying number placed on the vial with a marker pen.
- 10.16.2 All samples, QC aliquots, and one similar vial containing 25  $\mu\text{g}$  of  $\text{Cl}^-$  (irradiation standard) are then introduced into the reactor, generally by placing them together in a 5-dram polyethylene vial and inserting them into a pneumatic-tube transfer "rabbit" for neutron irradiation. Irradiation is typically for a 15 minute period at a thermal neutron irradiation flux of  $5 \times 10^{12}$  neutrons/cm<sup>2</sup>/sec. After returning from the reactor, the rabbit is allowed to "cool" for 20 minutes to allow short-lived interfering radioisotopes (primarily Al) present in the sample to decay.
- 10.16.3 Analyze each "cooled" vial beginning with the 25  $\mu\text{g}$  standard (Section 10.16.2) by counting the 1642-KeV gamma ray produced by  $^{38}\text{Cl}$ .  $^{38}\text{Cl}$  has a half-life of 37.1 minutes. The analyses can be performed either manually, with the operator changing samples and transferring the data to magnetic tape, or automatically, with both functions performed by an automatic sample changer.
- 10.16.4 Count the standard and samples for a suitable time period (e.g., 200 second "live " time for the standard and samples). The operator records the time intervals between samples and the "dead" time of each sample in a logbook for later use in calculating halogen concentrations in each sample.

10.16.5 Sample results are calculated per Section 12.

## 11.0 System and Laboratory Performance

- 11.1 At the beginning and end of each analytical sequence (each irradiation batch), system performance and calibration are verified. System performance and calibration verification may be performed more frequently, if desired.
- 11.1.1 If performance and calibration are verified at the beginning and end of each analytical sequence (or more frequently), samples analyzed during that period are considered valid.
- 11.1.2 If performance and calibration are not verified at the beginning and end of each analytical sequence (or more frequently), samples analyzed during that period must be re-analyzed.
- 11.1.3 If calibration is verified at the beginning of the analytical sequence, re-calibration is not necessary; otherwise, the instrument must be calibrated prior to analyzing samples.
- 11.2 Calibration Verification and Ongoing Precision and Recovery—Calibration and system performance are verified by the analysis of the 10 µg PAR standard.
- 11.2.1 Analyze the PAR standard (Section 6.12.3) and analyze a blank (Section 8.4) immediately thereafter at the beginning and end of each analytical sequence. Compute the concentration of organic halide in the PAR standard and in the blank. The blank shall be less than 2 µg Cl.
- 11.2.2 Subtract the result for the blank from the result of the PAR standard, and compute the percent recovery of the blank-subtracted PAR standard. The percent recovery shall be in the range of 71-116%.
- 11.2.3 If the recovery is within this range, the analytical process is in control and analysis of blanks and samples may proceed. If, however, the recovery is not within the acceptable range, the analytical process is not in control. In this event, correct the problem and repeat the on-going precision and recovery test (Section 11.2), or recalibrate (Sections 7.5 through 7.6).
- 11.2.4 If the recovery is not within the acceptable range for the PAR standard analyzed at the end of the analytical sequence, correct the problem, repeat the ongoing precision and recovery test (Section 11.2), or re-calibrate (Sections 7.5 through 7.6), and re-analyze the sample set that was analyzed during the analytical sequence.
- 11.3 Add results that pass the specification in Section 11.2.2 to initial and previous ongoing data. Update QC charts to form a graphic representation of continued laboratory performance. Develop a statement of laboratory data quality for each analyte by calculating the average percent recovery ( $R$ ) and the standard deviation of percent recovery ( $s_r$ ). Express the accuracy as a recovery interval from  $R-2s_r$  to  $R+2s_r$ . For example, if  $R = 95\%$  and  $s_r = 5\%$ , the accuracy is 85-105%.

## 12.0 Calculations

12.1 Calculate the concentration of chloride in each vial as per the following:

$$\mu\text{g Chloride} = (\text{cts unk}/\text{cts std})(\text{counting time std}/\text{counting time unk})(\mu\text{g in std})(e^{ht})$$

where,

cts unk = The integrated area of the appropriate gamma-ray peak in the sample with background subtracted and the total multiplied by  $1 + [(\% \text{ dead time unknown} - \% \text{ dead time std.})/200]$ . The latter correction is usually less than 4% and corrects for pile-up errors.

cts std = The integrated area of the appropriate gamma-ray peak in the standard with background subtracted.

counting time std = The "live" counting time in seconds of the standard.

counting time unk. = The "live" counting time in seconds of the unknown.

$\mu\text{g in std}$  = The number of micrograms of the stable element in the irradiation standard.

$e^{ht}$  = The decay correction to bring all statistics back to  $t = 0$ ;  $h = 0.693/t_{1/2}$ , where  $t_{1/2}$  is the half-life in minutes.

$t$  = The time interval in minutes from the end of the count of the irradiation standard until the end of the count of the sample.

12.1.1 All samples within an irradiation batch must be counted within two hours of irradiation.

12.1.2 If more than two hours pass after irradiation, the sample must be allowed to "cool" for 24 hours and then re-irradiated and re-analyzed with another batch of samples.

12.2 Calculate the concentration of chloride (in micrograms) detected in each sample per the following:

$$\text{OX (Cl)} (\mu\text{g}) = (C - B)$$

where,

C = Cl<sup>-</sup> from gamma-ray detector in a sample vial (Section 12.1),  $\mu\text{g}$ .

B = Cl<sup>-</sup> from gamma-ray detector in the beginning blank (Section 12.1),  $\mu\text{g}$ .

12.3 High Concentrations of OX—If the amount of chloride exceeds the calibration range, dilute the sample by a factor of 10 and re-analyze.

12.4 Low Concentrations of OX—The final result should be significantly (defined below) above the level of a blank.

12.4.1 If the instrument response of a sample exceeds the instrument response of the blank by a factor of at least 3, the result is acceptable.

12.4.2 If the instrument response of a sample is less than three times the instrument response of the blank, and the sample has been diluted, analyze a less dilute aliquot of sample.

- 12.4.3 If the instrument response of an undiluted sample is less than three times the instrument response of the blank, the result is suspect and may not be used for regulatory compliance purposes. In this case, find the cause of contamination, correct the problem, and re-analyze the sample under the corrected conditions.
- 12.5 Report final results that meet all of the specifications in this method as the blank-subtracted value, in  $\mu\text{g}/\text{L Cl}^-$  (not as 2,4,6-trichlorophenol), to three significant figures. This value is determined by subtracting the blank value determined in Section 8.4 from the value in Section 12.1.
- 13.0 Method Performance**—The specifications contained in this method are based on single laboratory data (Reference 13). These specification will be updated as further data become available.

## References

1. "Total Organic Halide, Methods 450.1 - Interim", Prepared by Stephen Billets and James J. Lichtenberg, USEPA, Office of Research and Development, Physical and Chemical Methods Branch, EMSL-Cincinnati, Cincinnati, OH 45268, EPA 600/4-81-056 (1981).
2. Method 9020, USEPA Office of Solid Waste, "Test Methods for Evaluating Solid Waste, SW-846", Third Edition, 1987.
3. "Determination of adsorbable organic halogens (AOX)", "German Standard Methods for the analysis of water, waste water and sludge -- General parameters of effects and substances", Deutsche Industrie Norm (DIN) Method 38 409, Part 14, DIN German Standards Institute, Beuth Verlag, Berlin, Germany (1987).
4. "Water quality - Determination of adsorbable organic halogens (AOX)", International Organization for Standard/Draft International Standardization (ISO/DIS) Method 9562 (1988).
5. "Organically bound chlorine by the AOX method", SCAN-W 9:89, Secretariat, Scandinavian Pulp, Paper and Board Testing Committee, Box 5604, S-11486, Stockholm, Sweden (1989).
6. Method 5320, "Dissolved Organic Halogen", from: "Standard Methods for the Examination of Water and Wastewater", 5320, American Public Health Association, 1015 15th St NW, Washington DC 20005 (1989).
7. "Canadian Standard Method for the Determination of Adsorbable Organic Halides (AOX) in Waters and Wastewaters", Environment Canada and The Canadian Pulp and Paper Association (1990).
8. 40 CFR Part 136, Appendix B (49 FR 43234; October 26, 1984).
9. "Working with Carcinogens," DHEW, PHS, CDC, NIOSH, Publication 77-206, (Aug 1977).



10. "OSHA Safety and Health Standards, General Industry" OSHA 2206, 29 CFR 1910 (Jan 1976).
11. "Safety in Academic Chemistry Laboratories," ACS Committee on Chemical Safety (1979).
12. "Methods 330.4 and 330.5 for Total Residual Chlorine," USEPA, EMSL Cincinnati, OH 45268, EPA-4-79-020 (March 1979).
13. "Validation of Method 1650: Determination of Organic Halide", Analytical Technologies Inc, ERCE Contract 87-3410, November 15, 1990. Available from the EPA Sample Control Center, Viar & Co, 300 N Lee St, Alexandria VA 22314 (703-557-5040).
14. Method 9022, USEPA Office of Solid Waste, "Test Methods for Evaluating Solid Waste, SW-846", Third Edition, 1987.