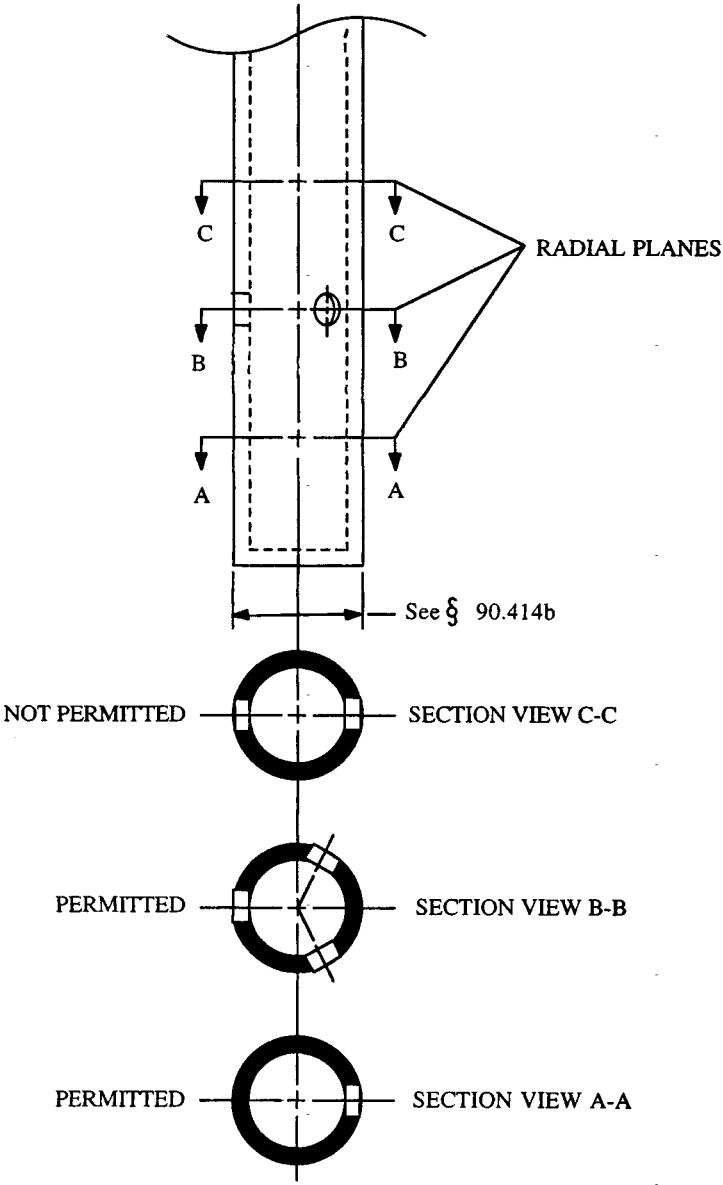


**Figure 2.--Sample Probe and Typical Hole Spacings**