

COLUMN: 1.5% SP-2250/1.95% SP-2401 ON SUPELCOPORT  
TEMPERATURE: 220°C  
DETECTOR: ELECTRON CAPTURE

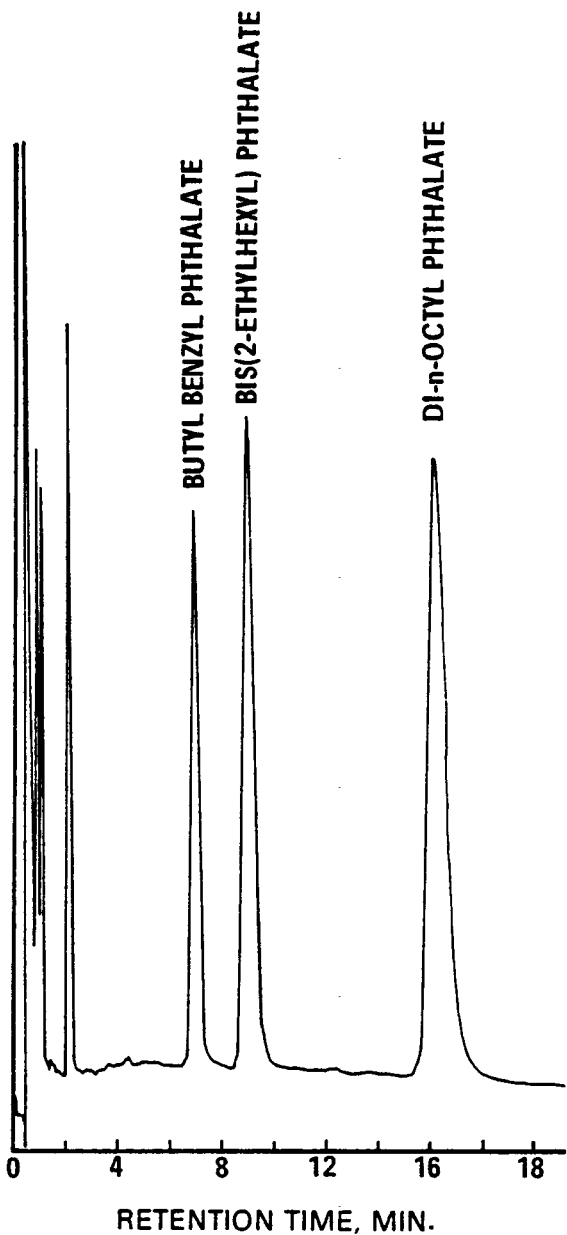


Figure 2. Gas chromatogram of phthalates.