

COLUMN: 1.5% SP-2250/1.95% SP-2401 ON SUPELCOPORT  
TEMPERATURE: 160°C.  
DETECTOR: ELECTRON CAPTURE

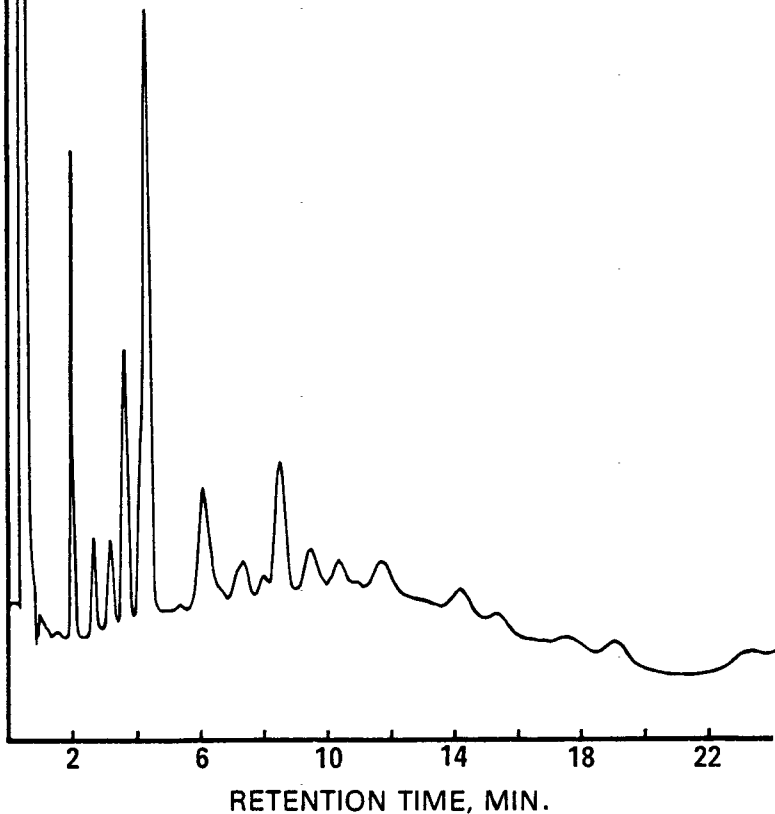


Figure 5. Gas chromatogram of PCB-1221.