

COLUMN: 1.5% SP-2250/1.95% SP-2401 ON SUPELCOPORT
TEMPERATURE: 160°C.
DETECTOR: ELECTRON CAPTURE

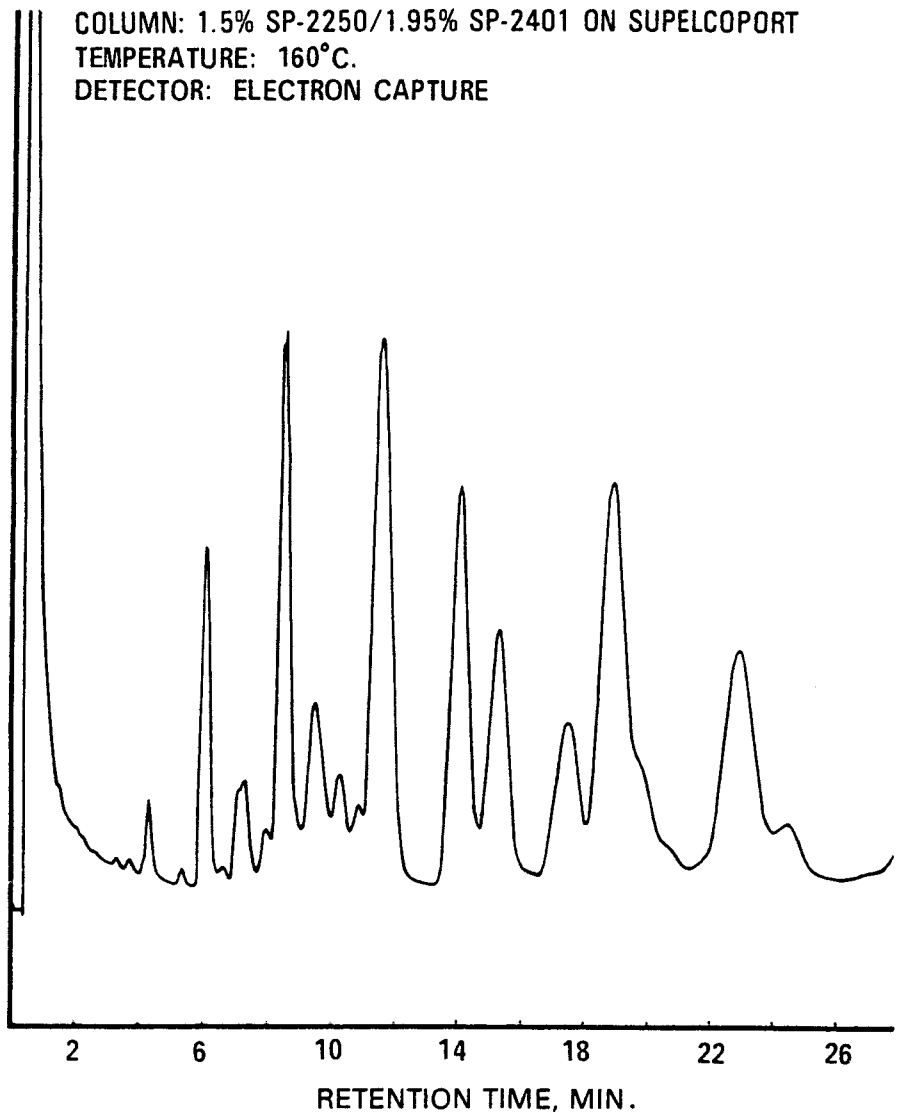


Figure 8. Gas chromatogram of PCB-1248.