

COLUMN: HC-ODS SIL-X  
MOBILE PHASE: 40% TO 100% ACETONITRILE  
IN WATER  
DETECTOR: FLUORESCENCE

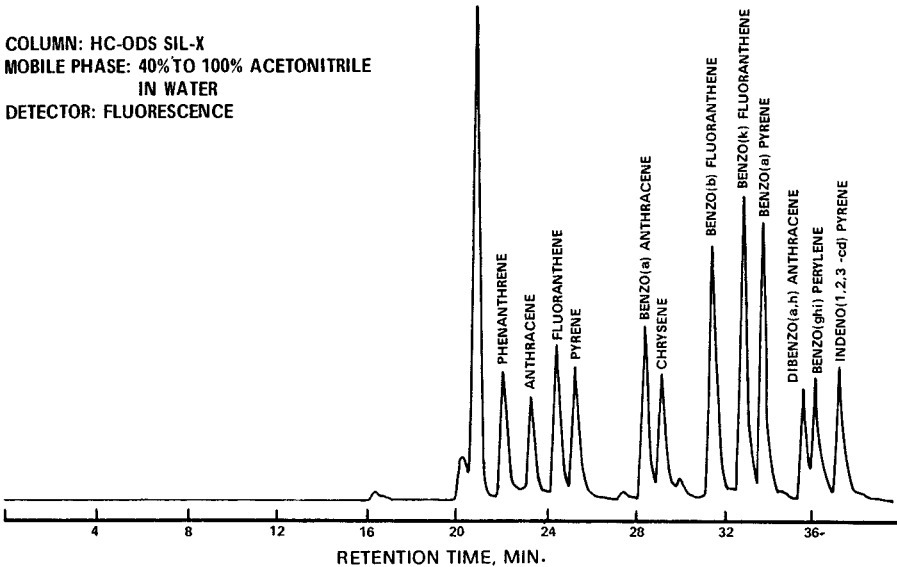


Figure 2. Liquid chromatogram of polynuclear aromatic hydrocarbons.