

COLUMN: 3% OV-17 ON CHROMOSORB W-AW-DCMS
PROGRAM: 100°C FOR 4 MIN, 8°C/MIN TO 280°C
DETECTOR: FLAME IONIZATION

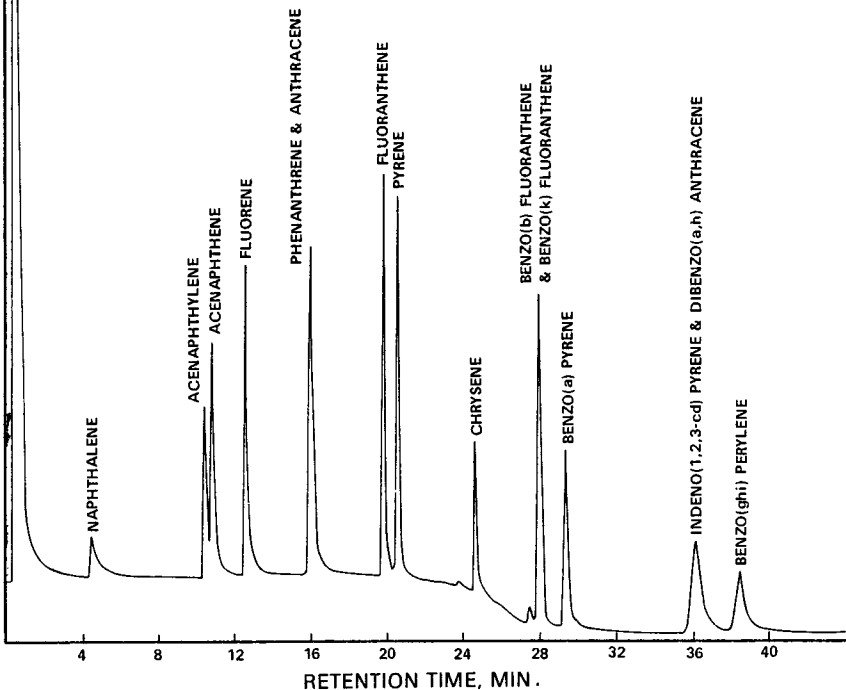


Figure 3. Gas chromatogram of polynuclear aromatic hydrocarbons.