

COLUMN: 1% SP-1000 ON CARBOPACK-B  
PROGRAM: 45°C FOR 3 MIN, 8°C/MIN TO 220°C  
DETECTOR: MASS SPECTROMETER

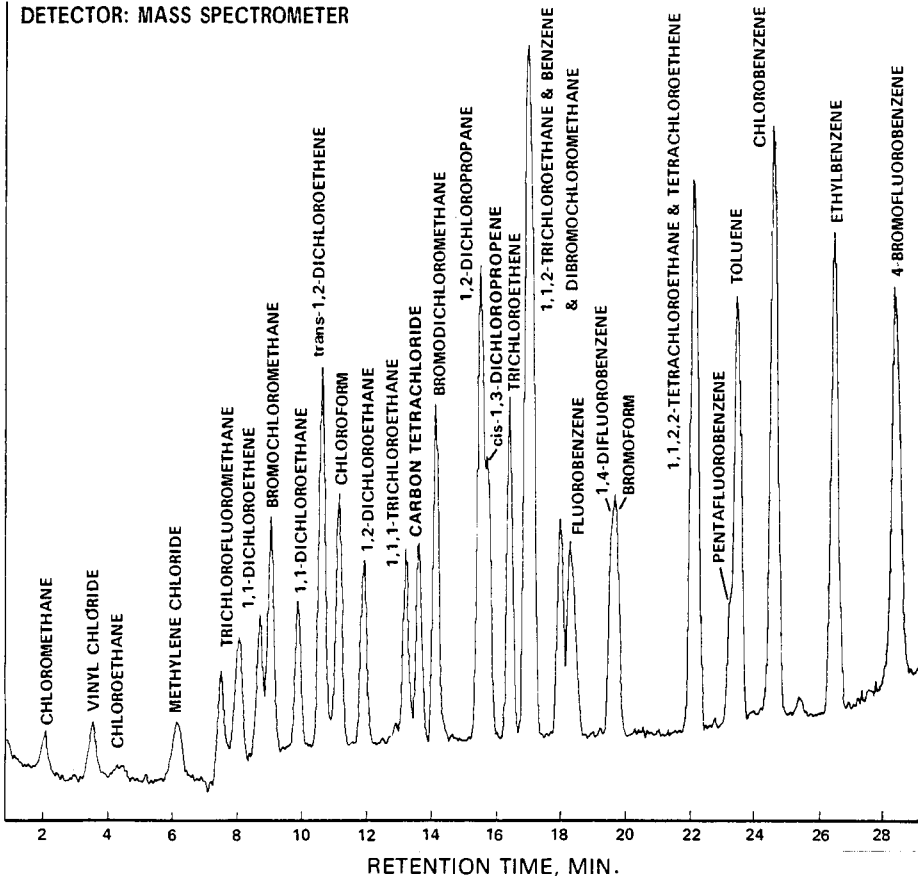


Figure 5. Gas chromatogram of volatile organics.