

COLUMN: 1% SP-1240DA ON SUPELCOPORT  
PROGRAM: 70°C FOR 2 MIN, 8°C/MIN TO 200°C  
DETECTOR: MASS SPECTROMETER.

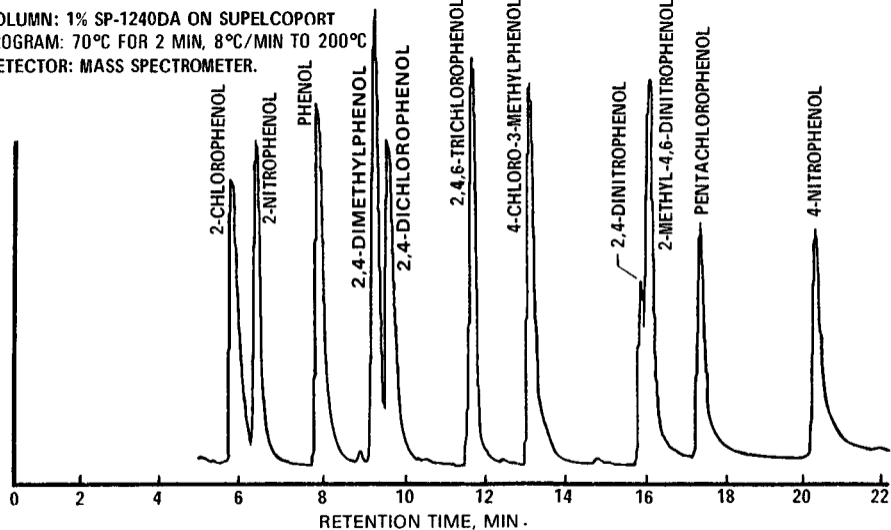


Figure 2. Gas chromatogram of acid fraction.