

COLUMN: 3% SP-2250 ON SUPELCOPORT  
PROGRAM: 50°C FOR 4 MIN, 8°C/MIN TO 270°C  
DETECTOR: MASS SPECTROMETER

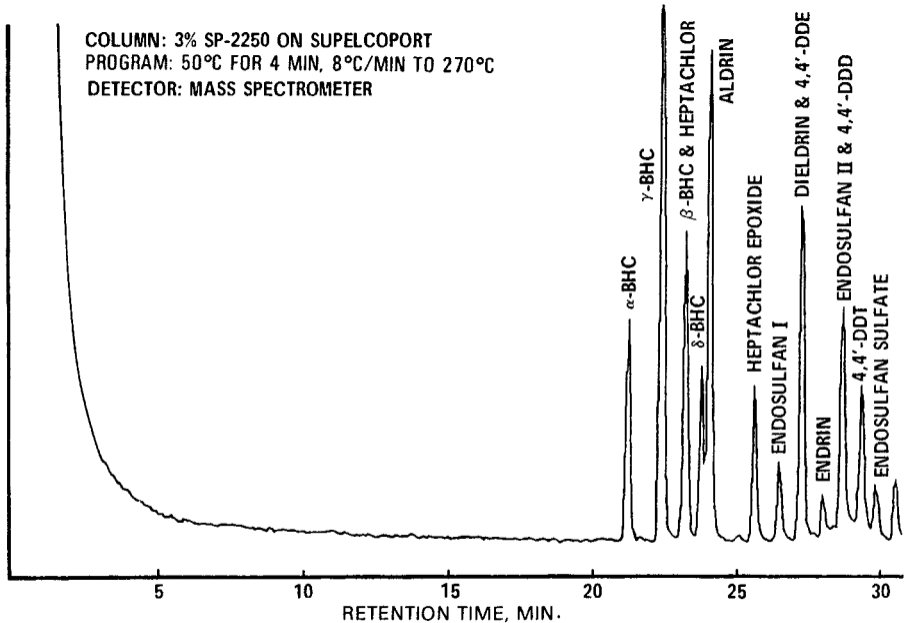


Figure 3. Gas chromatogram of pesticide fraction.