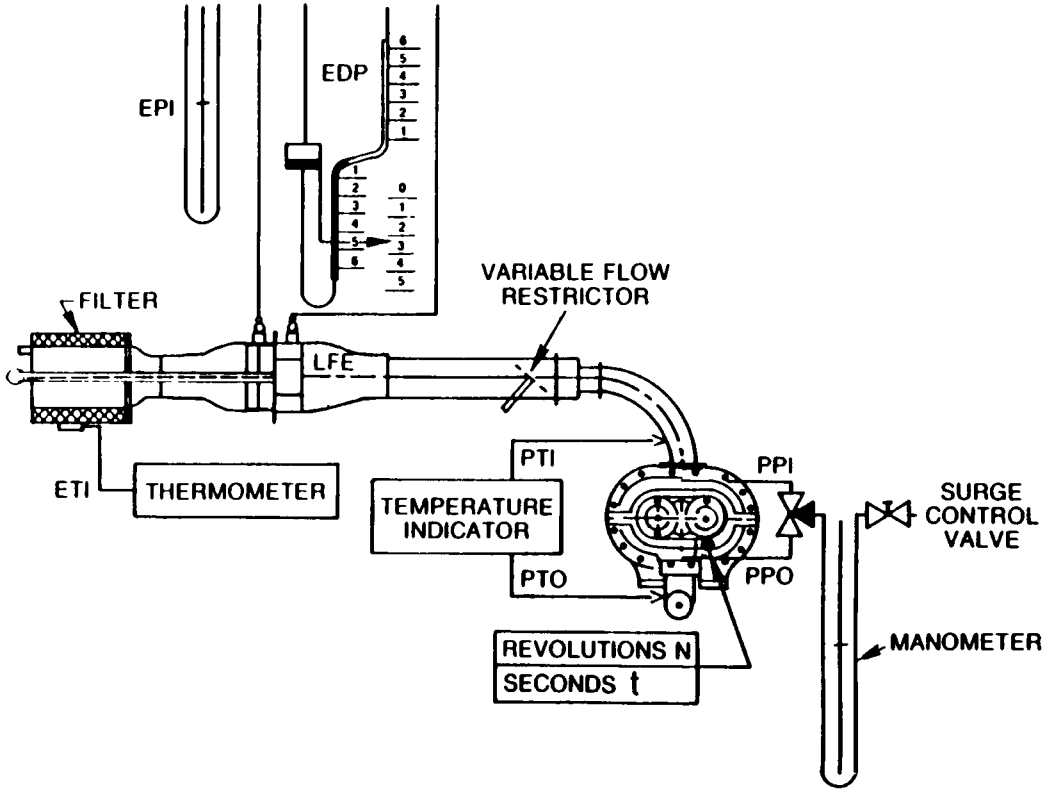

FIGURE B90-8 PDP-CVS CALIBRATION CONFIGURATION