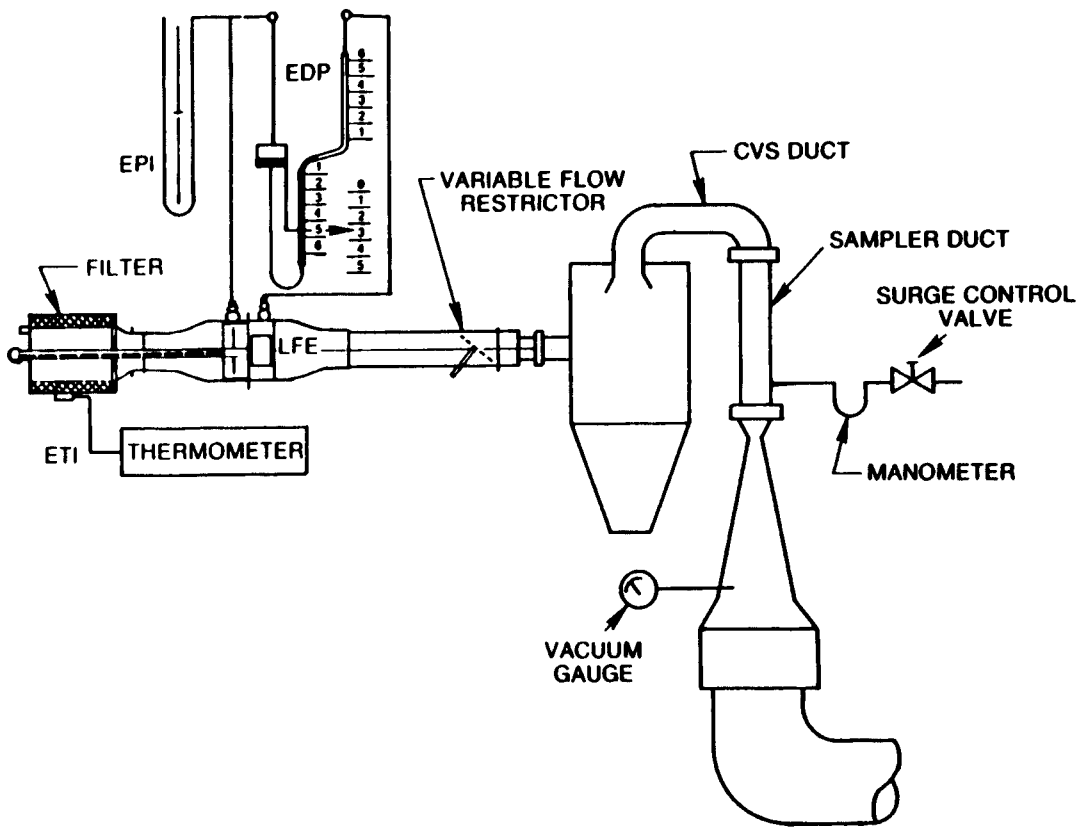

FIGURE B90-9 CFV-CVS CALIBRATION CONFIGURATION