

(e) The concentration of each test atmosphere shall be established and/or verified before or during each series of tests. Samples for verifying test concentrations shall be collected from the test atmosphere delivery system as close as possible to the sample intake port of the test analyzer.

(f) The accuracy of all flow measurements used to calculate test atmosphere concentrations shall be documented and referenced to a primary standard (such as a spirometer, bubble meter, etc.). Any corrections shall be clearly shown. All flow measurements given in volume units shall be standardized to 25 °C. and 760 mm Hg.

(g) Schematic drawings and other information showing complete procedural details of the test atmosphere generation, verification, and delivery system shall be provided. All pertinent calculations shall be clearly indicated.

[40 FR 7049, Feb. 18, 1975, as amended at 40 FR 18168, Apr. 25, 1975]

§ 53.23 Test procedures.

(a) *Range*—(1) *Technical definition.* Nominal minimum and maximum concentrations which a method is capable of measuring.

NOTE: The nominal range is specified at the lower and upper range limits in concentration units, for example, 0-0.5 p/m.

(2) *Test procedure.* Submit a suitable calibration curve, as specified in § 53.21(b), showing the test analyzer's response over at least 95 percent of the required range.

NOTE: A single calibration curve will normally suffice.

(b) *Noise*—(1) *Technical definition.* Spontaneous, short duration deviations in output, about the mean output, which are not caused by input concentration changes. Noise is determined as the standard deviation about the mean and is expressed in concentration units.

(2) *Test procedure.* (i) Allow sufficient time for the test analyzer to warm up and stabilize. Determine at two concentrations, first using zero air and then a pollutant test gas concentration as indicated below. The noise specification in table B-1 shall apply to both of these tests.

(ii) Connect an integrating-type digital meter (DM) suitable for the test analyzer's output and accurate to three significant digits, to measure the analyzer's output signal.

NOTE: Use of a chart recorder in addition to the DM is optional.

(iii) Measure zero air for 60 minutes. During this 60-minute interval, record twenty-five (25) readings at 2-minute intervals. (See Figure B-2 in appendix A.)

(iv) Convert each DM reading to concentration units (p/m) by reference to the test analyzer's calibration curve as determined in § 53.21(b). Label the converted DM readings $r_1, r_2, r_3 \dots r_i \dots r_{25}$.

(v) Calculate the standard deviation, S , as follows:

$$S = \sqrt{\frac{\sum_{i=1}^{25} (r_i)^2 - \frac{1}{25} \left(\sum_{i=1}^{25} r_i \right)^2}{24}} (p/m)$$

where i indicates the i -th DM reading in ppm.

(vi) Let S at 0 ppm be identified as S_0 ; compare S_0 to the noise specification given in table B-1.

(vii) Repeat steps (iii) through (vi) of this section using a pollutant test atmosphere concentration of 80±5 percent of the upper range limit (URL) instead of zero gas, and let S at 80 percent of the URL be identified as S_{80} . Compare S_{80} to the noise specification given in table B-1.

(viii) Both S_0 and S_{80} must be less than or equal to the specification for noise to pass the test for the noise parameter.

(c) *Lower detectable limit*—(1) *Technical definition.* The minimum pollutant concentration which produces a signal of twice the noise level.

(2) *Test procedure.* (i) Allow sufficient time for the test analyzer to warm up and stabilize. Measure zero air and record the stable reading in ppm as B_Z . (See Figure B-3 in appendix A.)

(ii) Generate and measure a pollutant test atmosphere concentration equal to the value for the lower detectable limit specified in table B-1.

NOTE: If necessary, the test atmosphere concentration may be generated or verified at a higher concentration, then accurately

§ 53.23

40 CFR Ch. I (7-1-04 Edition)

diluted with zero air to the final required concentration.

(iii) Record the test analyzer's stable indicated reading, in ppm, as B_L .

(iv) Determine the Lower Detectable Limit (LDL) as $LDL = B_L - B_Z$. Compare this LDL value with the noise level, S_0 , determined in § 53.23(b), for 0 concentration test atmosphere. LDL must be equal to or higher than $2S_0$ to pass this test.

(d) *Interference equivalent*—(1) *Technical definition*. Positive or negative response caused by a substance other than the one being measured.

(2) *Test procedure*. The test analyzer shall be tested for all substances likely to cause a detectable response. The test analyzer shall be challenged, in turn, with each interfering agent specified in table B-3. In the event that there are substances likely to cause a significant interference which have not been specified in table B-3, these substances shall be tested at a concentration substantially higher than that normally found in the ambient air. The

interference may be either positive or negative, depending on whether the test analyzer's response is increased or decreased by the presence of the interferent. Interference equivalents shall be determined by mixing each interferent, one at a time, with the pollutant at the concentrations specified in table B-3, and comparing the test analyzer's response to the response caused by the pollutant alone. Known gas-phase reactions that might occur between an interferent and the pollutant are designated by footnote 3 in table B-3. In these cases, the interference equivalent shall be determined in the absence of the pollutant.

(i) Allow sufficient time for warm-up and stabilization of the test analyzer.

(ii) For a candidate method using a prefilter or scrubber based upon a chemical reaction to derive part of its specificity, and which requires periodic service or maintenance, the test analyzer shall be "conditioned" prior to each interference test as follows:

TABLE B-3—INTERFERENT TEST CONCENTRATION,¹ PARTS PER MILLION

Pollutant	Analyzer type ²	Hydrochloric acid	Ammonia	Hydrogen sulfide	Sulfur dioxide	Nitrogen dioxide	Nitric oxide	Carbon dioxide	Ethylene	Ozone	M-xylene	Water vapor	Carbon monoxide	Methane	Ethane
SO ₂	Flame photometric (FPD)			0.1	1.0,14			750				320,000	50		
SO ₂	Gas chromatography (FPD)			.1	4,14			750				320,000	50		
SO ₂	Spectrophotometric-wet chemical (pararosaniline reaction)	0.2	3 0.1	.1	4,14	0.5		750		0.5					
SO ₂	Electrochemical	.2	3 1	.1	4,14	.5	0.5		0.2	.5		320,000			
SO ₂	Conductivity	.2	3 1		4,14	.5		750							
SO ₂	Spectrophotometric-gas phase				4,14	.5	.5				0.2				
O ₃	Chemiluminescent			3 1				750		4.08		320,000			
O ₃	Electrochemical			3 1	.5					4.08		320,000			
O ₃	Spectrophotometric-wet chemical (potassium iodide reaction)			3 1	.5	.5	3.5			4.08					
O ₃	Spectrophotometric-gas phase				.5	.5	3.5			4.08					
CO	Infrared							750				20,000	4 10		0.5
CO	Gas chromatography with flame ionization detector											20,000	4 10		
CO	Electrochemical						.5		.2			20,000	4 10	5.0	.5
CO	Catalytic combustion-thermal detection			.1				750	.2			20,000	4 10		
CO	IR fluorescence							750				20,000	4 10		.5
CO	Mercury replacement UV photometric								.2				4 10		.5
NO ₂	Chemiluminescent			3 1	.5	4.1	.5					20,000			
NO ₂	Spectrophotometric-wet chemical (azo-dye reaction)				.5	4.1	.5	750		.5					
NO ₂	Electrochemical	0.2	3 1		.5	4.1	.5	750		.5		20,000	50		
NO ₂	Spectrophotometric-gas phase		3 1		.5	4.1	.5			.5		20,000	50		

¹ Concentrations of interferent listed must be prepared and controlled to ± 10 percent of the state value.

² Analyzer types not listed will be considered by the administrator as special cases.

³ Do not mix with pollutant.

⁴ Concentration of pollutant used for test. These pollutant concentrations must be prepared to ± 10 percent of the stated value.

§ 53.23

40 CFR Ch. I (7-1-04 Edition)

(A) Service or perform the indicated maintenance on the scrubber or prefilter as directed in the manual referred to in § 53.4(b)(3).

(B) Before testing for each interferent, allow the test analyzer to sample through the scrubber a test atmosphere containing the interferent at a concentration equal to the value specified in table B-3. Sampling shall be at the normal flow rate and shall be continued for 6 continuous hours prior to testing.

(iii) Generate three test atmosphere streams as follows:

(A) Test atmosphere *P*: Pollutant concentration.

(B) Test atmosphere *I*: Interference concentration.

(C) Test atmosphere *Z*: Zero air.

(iv) Adjust the individual flow rates and the pollutant or interferent generators for the three test atmospheres as follows:

(A) The flow rates of test atmospheres *I* and *Z* shall be identical.

(B) The concentration of pollutant in test atmosphere *P* shall be adjusted such that when *P* is mixed (diluted) with either test atmosphere *I* or *Z*, the resulting concentration of pollutant shall be as specified in table B-3.

(C) The concentration of interferent in test atmosphere *I* shall be adjusted such that when *I* is mixed (diluted) with test atmosphere *P*, the resulting concentration of interferent shall be equal to the value specified in table B-3.

(D) To minimize concentration errors due to flow rate differences between *I* and *Z*, it is recommended that, when possible, the flow rate of *P* be from 10 to 20 times larger than the flow rates of *I* and *Z*.

(v) Mix test atmospheres *P* and *Z* by passing the total flow of both atmospheres through a mixing flask.

(vi) Sample and measure the mixture of test atmospheres *P* and *Z* with the test analyzer. Allow for a stable reading, and record the reading, in concentration units, as *R* (see Figure B-3).

(vii) Mix test atmospheres *P* and *I* by passing the total flow of both atmospheres through a mixing flask.

(viii) Sample and measure this mixture. Record the stable reading, in concentration units, as *R_I*.

(ix) Calculate the interference equivalent (*IE*) as:

$$IE = R_I - R$$

IE must be equal to or less than the specification given in table B-1 for each interferent to pass the test.

(x) Follow steps (iii) through (ix) of this section, in turn, to determine the interference equivalent for each interferent.

(xi) For those interferents which cannot be mixed with the pollutant, as indicated by footnote (3) in table B-3, adjust the concentration of test atmosphere *I* to the specified value without being mixed or diluted by the pollutant test atmosphere. Determine *IE* as follows:

(A) Sample and measure test atmosphere *Z* (zero air). Allow for a stable reading and record the reading, in concentration units, as *R*.

(B) Sample and measure the interferent test atmosphere *I*. If the test analyzer is not capable of negative readings, adjust the analyzer (not the recorder) to give an offset zero. Record the stable reading in concentration units as *R_I*, extrapolating the calibration curve, if necessary, to represent negative readings.

(C) Calculate $IE = R_I - R$. *IE* must be equal to or less than the specification in table B-1 to pass the test.

(xii) Sum the absolute value of all the individual interference equivalents. This sum must be equal to or less than the total interferent specification given in table B-1 to pass the test.

(e) *Zero drift, span drift, lag time, rise time, fall time, and precision*—(1) *Technical definitions*—(i) *Zero drift*: The change in response to zero pollutant concentration, over 12- and 24-hour periods of continuous unadjusted operation.

(ii) *Span drift*: The percent change in response to an up-scale pollutant concentration over a 24-hour period of continuous unadjusted operation.

(iii) *Lag time*: The time interval between a step change in input concentration and the first observable corresponding change in response.

(iv) *Rise time*: The time interval between initial response and 95 percent of final response after a step increase in input concentration.

Environmental Protection Agency

§ 53.23

(v) *Fall time:* The time interval between initial response and 95 percent of final response after a step decrease in input concentration.

(vi) *Precision:* Variation about the mean of repeated measurements of the same pollutant concentration, expressed as one standard deviation about the mean.

(2) Tests for these performance parameters shall be accomplished over a period of seven (7) or more days. During this time, the line voltage supplied to the test analyzer and the ambient temperature surrounding the analyzer shall be varied from day to day. One test result for each performance parameter shall be obtained each test day, for seven (7) or fifteen (15) test days as necessary. The tests are performed sequentially in a single procedure.

(3) The 24-hour test day may begin at any clock hour. The first 12 hours out of each test day are required for testing 12-hour zero drift. Tests for the other parameters shall be conducted during the remaining 12 hours.

(4) Table B-4 specifies the line voltage and room temperature to be used for each test day. The line voltage and temperature shall be changed to the specified values at the start of each test day (i.e., at the start of the 12-hour zero test). Initial adjustments (day zero) shall be made at a line voltage of 115 volts (rms) and a room temperature of 25 °C.

(5) The tests shall be conducted in blocks consisting of 3 test days each until 7 or 15 test results have been obtained. (The final block may contain fewer than three test days.) If a test is interrupted by an occurrence other

than a malfunction of the test analyzer, only the block during which the interruption occurred shall be repeated.

(6) During each block, manual adjustments to the electronics, gas, or reagent flows or periodic maintenance shall not be permitted. Automatic adjustments which the test analyzer performs by itself are permitted at any time.

(7) At least 4 hours prior to the start of the first test day of each block, the test analyzer may be adjusted and/or serviced according to the periodic maintenance procedures specified in the manual referred to in § 53.4(b)(3). If a new block is to immediately follow a previous block, such adjustments or servicing may be done immediately after completion of the day's tests for the last day of the previous block and at the voltage and temperature specified for that day, but only on test days 3, 6, 9, and 12.

NOTE: If necessary, the beginning of the test days succeeding such maintenance or adjustment may be delayed as necessary to complete the service or adjustment operation.

(8) All response readings to be recorded shall first be converted to concentration units according to the calibration curve. Whenever a test atmosphere is to be measured but a stable reading is not required, the test atmosphere shall be measured long enough to cause a change in response of at least 10% of full scale. Identify all readings and other pertinent data on the strip chart. (See Figure B-1 illustrating the pattern of the required readings.)

TABLE B-4—LINE VOLTAGE AND ROOM TEMPERATURE TEST CONDITIONS

Test day	Line voltage, ¹ rms	Room temperature, ² °C	Comments
0	115	25	Initial set-up and adjustments.
1	125	20	
2	105	20	
3	125	30	Adjustments and/or periodic maintenance permitted at end of tests.
4	105	30	
5	125	20	
6	105	20	Adjustments and/or periodic maintenance permitted at end of tests.
7	125	30	Examine test results to ascertain if further testing is required.
8	105	30	
9	125	20	Adjustments and/or periodic maintenance permitted at end of tests.
10	105	20	
11	125	30	
12	105	30	Adjustments and/or periodic maintenance permitted at end of tests.

§ 53.23

40 CFR Ch. I (7-1-04 Edition)

TABLE B-4—LINE VOLTAGE AND ROOM TEMPERATURE TEST CONDITIONS—Continued

Test day	Line voltage, ¹ rms	Room temperature, ² °C	Comments
13	125	20	
14	105	20	
15	125	30	

¹ Voltage specified shall be controlled to ± 1 volt.

² Temperature specified shall be controlled to ± 1 °C.

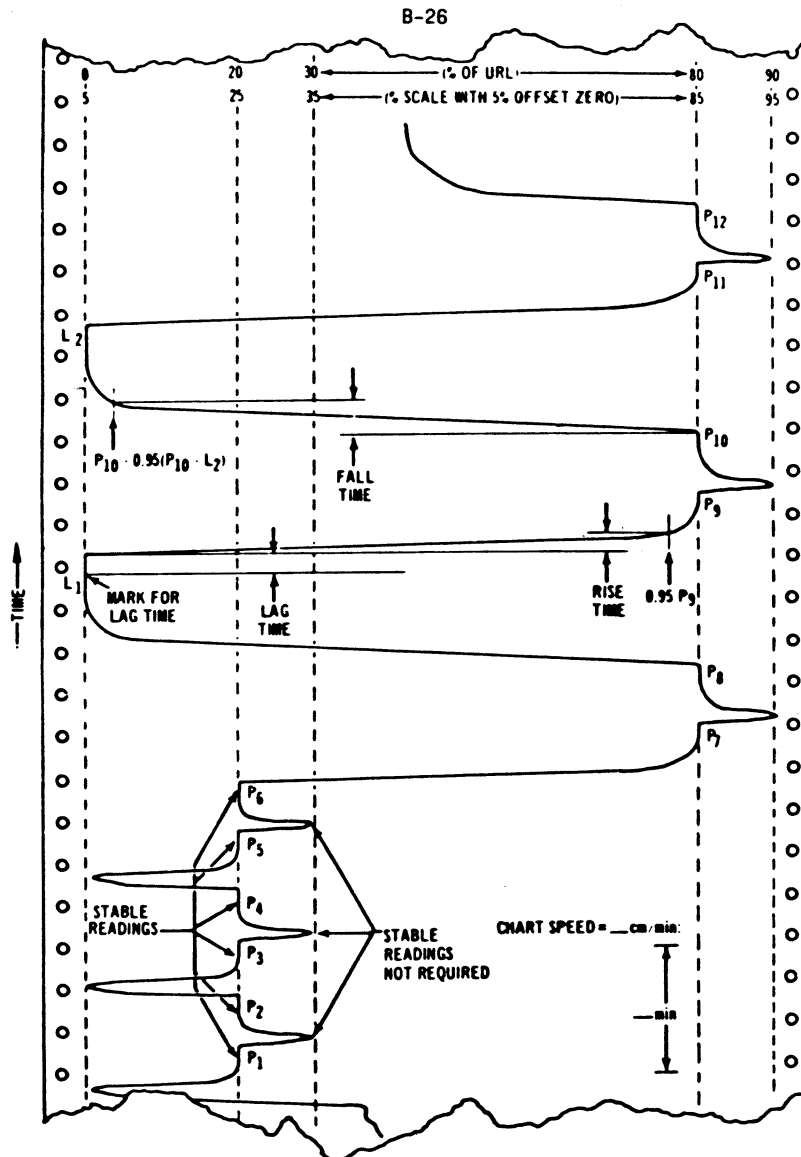


Figure B-1. Example showing the nature of the tracing obtained during the test for drift, lag time, rise time, fall time, and precision. The time scale has been greatly compressed.

(9) Test procedure. (i) Arrange to generate pollutant test atmospheres as follows:

Test atmosphere	Pollutant concentration (percent)
A ₀	Zero air.
A ₂₀	20±5 of the upper range limit.
A ₃₀	30±5 of the upper range limit.

§ 53.23

40 CFR Ch. I (7-1-04 Edition)

Test atmosphere	Pollutant concentration (percent)
A ₈₀	80±5 of the upper range limit.
A ₉₀	90±5 of the upper range limit.

Test atmospheres A₀, A₂₀, and A₈₀ shall be consistent during the tests and from day to day.

(ii) For steps (xxv) through (xxxi) of this section, a chart speed of at least 10 centimeters per hour shall be used. The actual chart speed, chart speed changes, and time checks shall be clearly marked on the chart.

(iii) Allow sufficient time for test analyzer to warm up and stabilize at a line voltage of 115 volts and a room temperature of 25 °C. Recalibrate, if necessary, and adjust the zero baseline to 5 percent of chart. No further adjustments shall be made to the analyzer until the end of the tests on the third day.

(iv) Measure test atmosphere A₀ until a stable reading is obtained, and record this reading (in ppm) as Z_n, where n = 0 (see Figure B-4 in appendix A).

(v) Measure test atmosphere A₂₀. Allow for a stable reading and record it as M_n, where n = 0.

(vi) Measure test atmosphere A₈₀. Allow for a stable reading and record it as S_n, where n = 0.

(vii) The above readings for Z₀, M₀, and S₀ should be taken at least four (4) hours prior to the beginning of test day 1.

(viii) At the beginning of each test day, adjust the line voltage and room temperature to the values given in table B-4.

(ix) Measure test atmosphere A₀ continuously for at least twelve (12) continuous hours during each test day.

(x) After the 12-hour zero drift test (step ix), sample test atmosphere A₀. A stable reading is not required.

(xi) Measure test atmosphere A₂₀ and record the stable reading (in ppm) as P₁. (See Figure B-4 in appendix A.)

(xii) Sample test atmosphere A₃₀; a stable reading is not required.

(xiii) Measure test atmosphere A₂₀ and record the stable reading as P₂.

(xiv) Sample test atmosphere A₀; a stable reading is not required.

(xv) Measure test atmosphere A₂₀ and record the stable reading as P₃.

(xvi) Sample test atmosphere A₃₀; a stable reading is not required.

(xvii) Measure test atmosphere A₂₀ and record the stable reading as P₄.

(xviii) Sample test atmosphere A₀; a stable reading is not required.

(xix) Measure test atmosphere A₂₀ and record the stable reading as P₅.

(xx) Sample test atmosphere A₃₀; a stable reading is not required.

(xxi) Measure test atmosphere A₂₀ and record the stable reading as P₆.

(xxii) Measure test atmosphere A₃₀ and record the stable reading as P₇.

(xxiii) Sample test atmosphere A₉₀; a stable reading is not required.

(xxiv) Measure test atmosphere A₈₀ and record the stable reading as P₈. Increase chart speed to at least 10 centimeters per hour.

(xxv) Measure test atmosphere A₀. Record the stable reading as L₁.

(xxvi) Quickly switch the test analyzer to measure test atmosphere A₈₀ and mark the recorder chart to show the exact time when the switch occurred.

(xxvii) Measure test atmosphere A₉₀ and record the stable reading as P₈₀.

(xxviii) Sample test atmosphere A₉₀; a stable reading is not required.

(xxix) Measure test atmosphere A₈₀ and record the stable reading as P₁₀.

(xxx) Measure test atmosphere A₀ and record the stable reading as L₂.

(xxxi) Measure test atmosphere A₈₀ and record the stable reading as P₁₁.

(xxxii) Sample test atmosphere A₉₀; a stable reading is not required.

(xxxiii) Measure test atmosphere A₈₀ and record the stable reading as P₁₂.

(xxxiv) Repeat steps (viii) through (xxxiii) of this section, each test day.

(xxxv) If zero and span adjustments are made after the readings are taken on test days 3, 6, 9, or 12, complete all adjustments; then measure test atmospheres A₀, A₈₀, and A₂₀. Allow for a stable reading on each, and record the readings as Z_nS_n, and M_n respectively, where n = the test day number.

(10) Determine the results of each day's tests as follows. Mark the recorder chart to show readings and determinations.

(i) *Zero drift.* (A) 12-hour. Examine the strip chart pertaining to the 12-

hour continuous zero air test. Determine the minimum (Cmin.) and maximum (Cmax.) readings (in p/m) during this period of 12 consecutive hours, extrapolating the calibration curve to negative concentration units if necessary. Determine the 12-hour zero drift (12ZD) as $12ZD = C_{max.} - C_{min.}$. (See Figure B-5 in appendix A.)

(B) Calculate the 24-hour zero drift (24ZD) for the n -th test day as $24ZD_n = Z_n - Z_{n-1}$, or $24ZD_n = Z_n - Z_{n-1}$ if zero adjustment was made on the previous day, where $Z_n = \frac{1}{2}(L_1 + L_2)$ for L_1 and L_2 taken on the n -th test day.

(C) Compare 12ZD and 24ZD to the zero drift specification in table B-1. Both 12ZD and 24ZD must be equal to or less than the specified value to pass the test for zero drift.

(ii) *Span drift.* (A) Span drift at 20 percent of URL (MSD)

$$MSD_n = \frac{M_n - M_{n-1}}{M_{n-1}} \times 100\%$$

$$MSD_n = \frac{M_n - M'_{n-1}}{M'_{n-1}} \times 100\%$$

If span adjustment was made on the previous day, where

$$M_n = \frac{1}{6} \sum_{i=1}^6 P_i$$

n indicates the n -th test day, and i indicates the i -th reading on the n th day.

(B) Span drift at 80 percent of URL (USD):

$$USD_n = \frac{S_n - S_{n-1}}{S_{n-1}} \times 100\%$$

or

$$USD_n = \frac{S_n - S'_{n-1}}{S'_{n-1}} \times 100\%$$

If span adjustment was made on the previous day, where

$$S_n = \frac{1}{6} \sum_{i=7}^{12} P_i$$

n indicates the n -th test day, and i indicates the i -th reading on the n -th test day.

(C) Both USD and MSD must be equal to or less than the respective specifications given in table B-1 to pass the test for span draft.

(iii) *Lag time.* Determine, from the strip chart, the elapsed time in minutes between the mark made in step (xxvi) and the first observable (two times the noise level) response. This time must be equal to or less than the time specified in table B-1 to pass the test for lag time.

(iv) *Rise time.* Calculate 95 percent of reading P_9 and determine from the recorder chart, the elapsed time between the first observable (two times noise level) response and a response equal to 95 percent of the P_9 reading. This time must be equal to or less than the rise time specified in table B-1 to pass the test for rise time.

(v) *Fall time.* Calculate five percent of ($P_{10} - L_2$) and determine, from the strip chart, the elapsed time in minutes between the first observable decrease in response following reading P_{10} and a response equal to five percent of ($P_{10} - L_2$). This time must be equal to or less than the fall time specification in table B-1 to pass the test for fall time.

(vi) *Precision.* Calculate precision (P_{20} and P_{80}) for each day's test as follows: (A)

$$P_{30} = \sqrt{\frac{1}{5} \left[\sum_{i=1}^6 P_i^2 - \frac{1}{6} \left(\sum_{i=1}^6 P_i \right)^2 \right]}$$

(B)

$$P_{30} = \sqrt{\frac{1}{5} \left[\sum_{i=7}^{12} P_i^2 - \frac{1}{6} \left(\sum_{i=7}^{12} P_i \right)^2 \right]}$$

(C) Both P_{20} and P_{80} must be equal to or less than the specification given in table B-1 to pass the test for precision.

[40 FR 7049, Feb. 18, 1975, as amended at 41 FR 52694, Dec. 1, 1976]

Pt. 53, Subpt. B, App. A

40 CFR Ch. I (7-1-04 Edition)

**APPENDIX A TO SUBPART B OF PART 53—
OPTIONAL FORMS FOR REPORTING
TEST RESULTS**

**TABLE B-5—SYMBOLS AND ABBREVIATIONS—
Continued**

TABLE B-5—SYMBOLS AND ABBREVIATIONS

B_L	Analyzer reading at specified <i>LDL</i> concentration.	P_{20}	Precision at 20 percent of <i>URL</i> .
B_z	Analyzer reading at 0 concentration for <i>LDL</i> test.	P_{80}	Precision at 80 percent of <i>URL</i> .
<i>DM</i>	Digital meter.	<i>R</i>	Analyzer reading of pollutant alone for <i>IE</i> test.
C_{max}	Maximum analyzer reading during 12ZD test.	R_I	Analyzer reading with interferent added for <i>IE</i> test.
C_{min}	Minimum analyzer reading during 12ZD test.	r_i	The <i>i</i> -th <i>DM</i> reading for noise test.
<i>i</i>	Subscript indicating the <i>i</i> -th quantity in a series.	<i>S</i>	Standard deviation of noise readings.
<i>IE</i>	Interference equivalent.	S_0	Noise value (<i>S</i>) measured at 0 concentration.
L_1	First analyzer zero reading for 24ZD test.	S_{80}	Noise value (<i>S</i>) measured at 80 percent of <i>URL</i> .
L_2	Second analyzer zero reading for 24ZD test.	S_n	Average of $P_7 \dots P_{12}$ for the <i>n</i> -th test day.
M_n	Average of $P_1 \dots P_6$ for the <i>n</i> -th test day.	S'_n	Adjusted span reading at 80 percent of <i>URL</i> on the <i>n</i> -th test day.
M'_n	Adjusted span reading at 20 percent of <i>URL</i> on the <i>n</i> -th test day.	<i>URL</i>	Upper range limit.
<i>MSD</i>	Span drift at 20 percent of <i>URL</i> .	<i>USD</i>	Span drift at 80 percent of <i>URL</i> .
<i>n</i>	Subscript indicating the test day number.	<i>Z</i>	Average of L_1 and L_2 .
<i>P</i>	Analyzer reading for precision test.	Z_n	Average of L_1 and L_2 on the <i>n</i> -th test day.
P_i	The <i>i</i> -th analyzer reading for precision test.	Z'_n	Adjusted zero reading on the <i>n</i> -th test day.
		<i>ZD</i>	Zero drift.
		12ZD	12-hour zero drift.
		24ZD	24-hour zero drift.

Environmental Protection Agency

Pt. 53, Subpt. B, App. A

Applicant _____ Date _____

Test No. _____

Analyzer _____ Range _____

READING NUMBER (i)	TIME	0% of URL		80% of URL	
		DM READING	r_i , ppm	DM READING	r_i , ppm
1					
2					
3					
4					
5					
6					
7					
8					
9					
10					
11					
12					
13					
14					
15					
16					
17					
18					
19					
20					
21					
22					
23					
24					
25					
$\sum_{i=1}^{25} r_i$					
$\sum_{i=1}^{25} r_i^2$					
S			$S_0 =$		$S_{80} =$

Figure B-2. Form for noise data.

Applicant _____		Range _____														
Analyzer _____		TEST NUMBER														
TEST PARAMETER	READING OR CALCULATION	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15
LOWER DETECTABLE LIMIT	B_2															
	B_L															
	$LDL = B_L - B_2$															
INTERFERENCE EQUIVALENT	R_1															
	R_{11}															
	$IE_1 = R_{11} \cdot R_1$															
	R_2															
	R_{12}															
	$IE_2 = R_{12} \cdot R_2$															
	R_3															
	R_{13}															
	$IE_3 = R_{13} \cdot R_3$															
	R_4															
	R_{14}															
	$IE_4 = R_{14} \cdot R_4$															
	R_5															
	R_{15}															
	$IE_5 = R_{15} \cdot R_5$															
TOTAL	$IE_T = \sum_{i=1}^5 IE_i$															

Figure B-3. Form for data and calculations for lower detectable limit and interference equivalent.

Applicant _____
 Analyzer _____ Range _____

TEST DAY (m)	ANALYZER READING, ppm															
DATE	0	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15
P ₁																
P ₂																
P ₃																
P ₄																
P ₅																
P ₆																
$\sum_{i=1}^6 P_i^2$																
P ₇																
P ₈																
P ₉																
P ₁₀																
P ₁₁																
P ₁₂																
$\sum_{i=7}^{12} P_i^2$																
L ₁																
L ₂																
Z _i																
M _i																
S _i																
C _{max}																
C _{min}																

Figure B-4. Form recording data for drift and precision.

Applicant		Range														
Analyzer		n -th TEST DAY														
TEST PARAMETER	CALCULATION	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15
Zero drift	12ZD = $C_{max} - C_{min}$															
	$Z = \frac{1}{2}(L_1 + L_2)$															
24 hour	24ZD = $Z_n - Z_{n-1}$															
	24ZD _n = $Z_n - Z'_{n-1}$															
20% URL	$M_n = \frac{1}{6} \sum_{i=1}^6 P_i$															
	$MSD_n = \frac{M_n - M_{n-1}}{M_{n-1}} \times 100\%$															
	$MSD_n = \frac{M'_n - M'_{n-1}}{M'_{n-1}} \times 100\%$															
Span drift	$S_n = \frac{1}{6} \sum_{i=7}^{12} P_i$															
	$USD_n = \frac{S_n - S_{n-1}}{S_{n-1}} \times 100\%$															
80% URL	$USD_n = \frac{S'_n - S'_{n-1}}{S'_{n-1}} \times 100\%$															
	$P_{20} = \sqrt{\frac{1}{5} \left[\sum_{i=1}^6 P_i^2 - \frac{1}{6} \left(\sum_{i=1}^6 P_i \right)^2 \right]}$															
Precision	$P_{80} = \sqrt{\frac{1}{5} \left[\sum_{i=7}^{12} P_i^2 - \frac{1}{6} \left(\sum_{i=7}^{12} P_i \right)^2 \right]}$															

Figure B-5. Form for calculating zero drift, span drift and precision.

Applicant _____		Analyst _____															
Analyzer _____		Range _____															
PERFORMANCE PARAMETER	Table B-1 spec.	TEST										No. of test failures	Pass or fail				
		1	2	3	4	5	6	7	8	9	10			11	12	13	14
NOISE, ppm	0% URL (S ₀)																
	80% URL (S ₈₀)																
LDL (must be 2 × noise)																	
INTER-FERENCE EQUIV. ALENT, ppm	IE ₁																
	IE ₂																
	IE ₃																
	IE ₄																
	IE ₅																
TOTAL (IE _T)																	
ZERO DRIFT, ppm	12 hour (1ZZD)																
	24 hour (2AZD)																
SPAN DRIFT, %	20% URL (MSD)																
	80% URL (USD)																
LAG TIME, min																	
RISE TIME, min																	
FALL TIME, min																	
PRECISION, ppm	20% URL (P ₂₀)																
	80% URL (P ₈₀)																

^aCompare each test LDL reading with the corresponding noise measurements. LDL reading must exceed the 0% URL noise value by a factor of 2 to pass the test for LDL.

Figure B-6. Form for summary of test results.

[40 FR 7049, Feb. 18, 1975, as amended at 40 FR 18169, Apr. 25, 1975]

Subpart C—Procedures for Determining Comparability Between Candidate Methods and Reference Methods

SOURCE: 62 FR 38792, July 18, 1997, unless otherwise noted.

§ 53.30 General provisions.

(a) *Determination of comparability.* The test procedures prescribed in this subpart shall be used to determine if a candidate method is comparable to a reference method when both methods measure pollutant concentrations in ambient air.