



National Institute for Occupational Safety and Health
National Personal Protective Technology Laboratory
P.O. Box 18070
Pittsburgh, PA 15236

Procedure No. RCT-ASR-STP-0137	Revision: 1.1	Date: 27 September 2005
--------------------------------	---------------	-------------------------

DETERMINATION OF CONTINUOUS GAS FLOW ON CONSTANT FLOW WITH DEMAND,
CLOSED-CIRCUIT, SELF-CONTAINED BREATHING APPARATUS
STANDARD TESTING PROCEDURE (STP)

1. PURPOSE

This test establishes the procedures for ensuring that the level of protection provided by the gas flow requirements on Constant Flow with Demand, Closed-Circuit, Self-Contained Breathing Apparatus (SCBA) submitted for Approval, Extension of Approval, or examined during Certified Product Audits, meet the minimum certification standards set forth in 42 CFR, Part 84, Subpart G, Section 84.63(a)(c)(d), and Subpart H, Section 84.94(b); Volume 60, Number 110, June 8, 1995.

2. GENERAL

This STP describes the Determination of Continuous Gas Flow on Constant Flow with Demand, Closed-Circuit, Self-Contained Breathing Apparatus test in sufficient detail that a person knowledgeable in the appropriate technical field can select equipment with the necessary resolution, conduct the test, and determine whether or not the product passes the test.

3. EQUIPMENT/MATERIALS

3.1. The list of necessary test equipment and materials follows:



3.1.1. Electric Timer, calibrated to hundredths of a minute (Precision Scientific Company) or equivalent.

Approvals:	<u>1st</u> Level	<u>2nd</u> Level	<u>3rd</u> Level
------------	------------------	------------------	------------------



- 3.1.2. Dry test - Gas meter, (Singer-American Meter Division - Model DTM-200A) or equivalent.



- 3.1.3. Wet Test - Gas Meter (Singer-American Meter Company - Model AL17-1) or equivalent.

4. TESTING REQUIREMENTS AND CONDITIONS

- 4.1. Prior to beginning any testing, all measuring equipment to be used must have been calibrated in accordance with the manufacturer's calibration procedure and schedule. At a minimum, all measuring equipment utilized for this testing must have been calibrated within the preceding 12 months using a method traceable to the National Institute of Standards and Technology (NIST).
- 4.2. The compressed gas cylinder must meet all applicable Department of Transportation requirements for cylinder approval as well as for retesting/requalification.
- 4.3. Normal laboratory safety practices must be observed. This includes all safety precautions described in the current ALOSH Facility Laboratory Safety Manual.
- 4.3.1. Safety glasses, lab coats, and hard-toe shoes must be worn at all times.
- 4.3.2. Work benches must be maintained free of clutter and non-essential test equipment.
- 4.3.3. When handling any glass laboratory equipment, lab technicians and personnel must wear special gloves which protect against lacerations or punctures.

5. PROCEDURE

Note: Reference Section 3 for equipment, model numbers and manufacturers. For calibration

purposes use those described in the manufacturer's operation and maintenance manuals.

- 5.1. The regulator or constant flow outlet is connected to a calibrated wet test meter (traceable to NIST using Dry Test Gas Meter).
- 5.2. Flow readings are recorded initially and every 10 minutes for the rated service time of the unit. The last 10 minutes are monitored every other minute.
- 5.3. Data Analysis

Record flow readings directly from the wet test gas meter.

Note: This test should be done on a minimum of two respirators, or more if additional testing is required (42 CFR, Part 84, Sections 84.12, 84.30, and 84.60).

6. PASS\FAIL CRITERIA

- 6.1. The criterion for passing this test is set forth in 42 CFR, Part 84, Subpart G, Section 84.63(a)(c)(d), and Subpart H, Section 84.94(b); Volume 60, Number 110, June 8, 1995.
- 6.2. This test establishes the standard procedure for ensuring that:

84.63 Test requirements; general.

(a) Each respirator and respirator component shall when tested by the applicant and by the Institute, meet the applicable requirements set forth in subparts H through L of this part.

(c) In addition to the minimum requirements set forth in subparts H through L of this part, the Institute reserves the right to require, as a further condition of approval, any additional requirements deemed necessary to establish the quality, effectiveness, and safety of any respirator used as protection against hazardous atmospheres.

(d) Where it is determined after receipt of an application that additional requirements will be required for approval, the Institute will notify the applicant in writing of these additional requirements, and necessary examinations, inspections, or tests, stating generally the reasons for such requirements, examinations, inspections, or tests.

84.94 Gas flow test; closed-circuit apparatus.

(b) Where constant flow is used in conjunction with demand flow, the constant flow shall be greater than 1.5 liters per minute for the entire rated service time.

7. RECORDS\TEST SHEETS

- 7.1. All test data will be recorded on the GAS FLOW TEST, CONSTANT FLOW WITH DEMAND, CLOSED-CIRCUIT, SELF-CONTAINED BREATHING APPARATUS test data sheet.

Procedure No. RCT-ASR-STP-0137	Revision: 1.1	Date: 27 September 2005	Page 4 of 13
--------------------------------	---------------	-------------------------	--------------

- 7.2. All videotapes and photographs of the actual test being performed, or of the test equipment shall be maintained in the task file as part of the permanent record.
- 7.3. All equipment failing any portion of this test will be handled as follows;
 - 7.3.1. If the failure occurs on a new certification application, or extension of approval application, send a test report to the RCT Leader and prepare the hardware for return to the manufacturer.
 - 7.3.2. If the failure occurs on hardware examined under an Off-the-Shelf Audit the hardware will be examined by a technician and the RCT Leader for cause. All equipment failing any portion of this test may be sent to the manufacturer for examination and then returned to NIOSH. However, the hardware tested shall be held at the testing laboratory until authorized for release by the RCT Leader, or his designee, following the standard operating procedures outlined in Procedure for Scheduling, and Processing Post-Certification Product Audits, RB-SOP-0005-00.

**GAS FLOW TEST, CONSTANT FLOW WITH DEMAND, CLOSED-CIRCUIT,
SELF-CONTAINED BREATHING APPARATUS**

Project No. : _____ Date: _____

Company : _____

Respirator Type: _____

Reference: 42 CFR 84, Subpart H, Section 84.94(b).

Requirement: Where constant flow is used in conjunction with demand flow, the constant flow shall be 1.5 lpm for entire rated service time of unit.

Results:

<u>Unit #1</u>	<u>Time/Min.</u>	<u>Flow/LPM</u>	<u>Unit #2</u>	<u>Time/Min.</u>	<u>Flow/LPM</u>
	0-1	_____		0-1	_____
	1-2	_____		1-2	_____
	2-3	_____		2-3	_____
	3-4	_____		3-4	_____
	4-5	_____		4-5	_____
	5-6	_____		5-6	_____
	6-7	_____		6-7	_____
	7-8	_____		7-8	_____
	8-9	_____		8-9	_____
	9-10	_____		9-10	_____
	10-11	_____		10-11	_____
	11-12	_____		11-12	_____
	12-13	_____		12-13	_____
	13-14	_____		13-14	_____
	14-15	_____		14-15	_____
	15-16	_____		15-16	_____
	16-17	_____		16-17	_____
	17-18	_____		17-18	_____
	18-19	_____		18-19	_____
	19-20	_____		19-20	_____
	20-21	_____		20-21	_____
	21-22	_____		21-22	_____
	22-23	_____		22-23	_____
	23-24	_____		23-24	_____
	24-25	_____		24-25	_____
	25-26	_____		25-26	_____
	26-27	_____		26-27	_____
	27-28	_____		27-28	_____
	28-29	_____		28-29	_____
	29-30	_____		29-30	_____

30-31	_____	30-31	_____
31-32	_____	31-32	_____
32-33	_____	32-33	_____
33-34	_____	33-34	_____
34-35	_____	34-35	_____
35-36	_____	35-36	_____
36-37	_____	36-37	_____
37-38	_____	37-38	_____
38-39	_____	38-39	_____
39-40	_____	39-40	_____
40-41	_____	40-41	_____
41-42	_____	41-42	_____
42-43	_____	42-43	_____
43-44	_____	43-44	_____
44-45	_____	44-45	_____
45-46	_____	45-46	_____
46-47	_____	46-47	_____
47-48	_____	47-48	_____
48-49	_____	48-49	_____
49-50	_____	49-50	_____
50-51	_____	50-51	_____
51-52	_____	51-52	_____
52-53	_____	52-53	_____
53-54	_____	53-54	_____
54-55	_____	54-55	_____
55-56	_____	55-56	_____
56-57	_____	56-57	_____
57-58	_____	57-58	_____
58-59	_____	58-59	_____
59-60	_____	59-60	_____
60-61	_____	60-61	_____
61-62	_____	61-62	_____
62-63	_____	62-63	_____
63-64	_____	63-64	_____
64-65	_____	64-65	_____
65-66	_____	65-66	_____
66-67	_____	66-67	_____
67-68	_____	67-68	_____
68-69	_____	68-69	_____
69-70	_____	69-70	_____
70-71	_____	70-71	_____
71-72	_____	71-72	_____
72-73	_____	72-73	_____
73-74	_____	73-74	_____
74-75	_____	74-75	_____
75-76	_____	75-76	_____
76-77	_____	76-77	_____
77-78	_____	77-78	_____

78-79	_____	78-79	_____
79-80	_____	79-80	_____
80-81	_____	80-81	_____
81-82	_____	81-82	_____
82-83	_____	82-83	_____
83-84	_____	83-84	_____
84-85	_____	84-85	_____
85-86	_____	85-86	_____
86-87	_____	86-87	_____
87-88	_____	87-88	_____
88-89	_____	88-89	_____
89-90	_____	89-90	_____
90-91	_____	90-91	_____
91-92	_____	91-92	_____
92-93	_____	92-93	_____
93-94	_____	93-94	_____
94-95	_____	94-95	_____
95-96	_____	95-96	_____
96-97	_____	96-97	_____
97-98	_____	97-98	_____
98-99	_____	98-99	_____
99-100	_____	99-100	_____
100-101	_____	100-101	_____
101-102	_____	101-102	_____
102-103	_____	102-103	_____
103-104	_____	103-104	_____
104-105	_____	104-105	_____
105-106	_____	105-106	_____
106-107	_____	106-107	_____
107-108	_____	107-108	_____
108-109	_____	108-109	_____
109-110	_____	109-110	_____
110-111	_____	110-111	_____
111-112	_____	111-112	_____
112-113	_____	112-113	_____
113-114	_____	113-114	_____
114-115	_____	114-115	_____
115-116	_____	115-116	_____
116-117	_____	116-117	_____
117-118	_____	117-118	_____
118-119	_____	118-119	_____
119-120	_____	119-120	_____
120-121	_____	120-121	_____
121-122	_____	121-122	_____
122-123	_____	122-123	_____
123-124	_____	123-124	_____
124-125	_____	124-125	_____
125-126	_____	125-126	_____


126-127	_____	126-127	_____
127-128	_____	127-128	_____
128-129	_____	128-129	_____
129-130	_____	129-130	_____
130-131	_____	130-131	_____
131-132	_____	131-132	_____
132-133	_____	132-133	_____
133-134	_____	133-134	_____
134-135	_____	134-135	_____
135-136	_____	135-136	_____
136-137	_____	136-137	_____
137-138	_____	137-138	_____
138-139	_____	138-139	_____
139-140	_____	139-140	_____
140-141	_____	140-141	_____
141-142	_____	141-142	_____
142-143	_____	142-143	_____
143-144	_____	143-144	_____
144-145	_____	144-145	_____
145-146	_____	145-146	_____
146-147	_____	146-147	_____
147-148	_____	147-148	_____
148-149	_____	148-149	_____
149-150	_____	149-150	_____
150-151	_____	150-151	_____
151-152	_____	151-152	_____
152-153	_____	152-153	_____
153-154	_____	153-154	_____
154-155	_____	154-155	_____
155-156	_____	155-156	_____
156-157	_____	156-157	_____
157-158	_____	157-158	_____
158-159	_____	158-159	_____
159-160	_____	159-160	_____
160-161	_____	160-161	_____
161-162	_____	161-162	_____
162-163	_____	162-163	_____
163-164	_____	163-164	_____
164-165	_____	164-165	_____
165-166	_____	165-166	_____
166-167	_____	166-167	_____
167-168	_____	167-168	_____
168-169	_____	168-169	_____
169-170	_____	169-170	_____
170-171	_____	170-171	_____
171-172	_____	171-172	_____
172-173	_____	172-173	_____
173-174	_____	173-174	_____


174-175	_____	174-175	_____
175-176	_____	175-176	_____
176-177	_____	176-177	_____
177-178	_____	177-178	_____
178-179	_____	178-179	_____
179-180	_____	179-180	_____
180-181	_____	180-181	_____
181-182	_____	181-182	_____
182-183	_____	182-183	_____
183-184	_____	183-184	_____
184-185	_____	184-185	_____
185-186	_____	185-186	_____
186-187	_____	186-187	_____
187-188	_____	187-188	_____
188-189	_____	188-189	_____
189-190	_____	189-190	_____
190-191	_____	190-191	_____
191-192	_____	191-192	_____
192-193	_____	192-193	_____
193-194	_____	193-194	_____
194-195	_____	194-195	_____
195-196	_____	195-196	_____
196-197	_____	196-197	_____
197-198	_____	197-198	_____
198-199	_____	198-199	_____
199-200	_____	199-200	_____
200-201	_____	200-201	_____
201-202	_____	201-202	_____
202-203	_____	202-203	_____
203-204	_____	203-204	_____
204-205	_____	204-205	_____
205-206	_____	205-206	_____
206-207	_____	206-207	_____
207-208	_____	207-208	_____
208-209	_____	208-209	_____
209-210	_____	209-210	_____
210-211	_____	210-211	_____
211-212	_____	211-212	_____
212-213	_____	212-213	_____
213-214	_____	213-214	_____
214-215	_____	214-215	_____
215-216	_____	215-216	_____
216-217	_____	216-217	_____
217-218	_____	217-218	_____
218-219	_____	218-219	_____
219-220	_____	219-220	_____
220-221	_____	220-221	_____
221-222	_____	221-222	_____

222-223	_____	222-223	_____
223-224	_____	223-224	_____
224-225	_____	224-225	_____
225-226	_____	225-226	_____
226-227	_____	226-227	_____
227-228	_____	227-228	_____
228-229	_____	228-229	_____
229-230	_____	229-230	_____
230-231	_____	230-231	_____
231-232	_____	231-232	_____
232-233	_____	232-233	_____
233-234	_____	233-234	_____
234-235	_____	234-235	_____
235-236	_____	235-236	_____
236-237	_____	236-237	_____
237-238	_____	237-238	_____
238-239	_____	238-239	_____
239-240	_____	239-240	_____

Comments :

Test Engineer: _____ PASS _____ FAIL _____

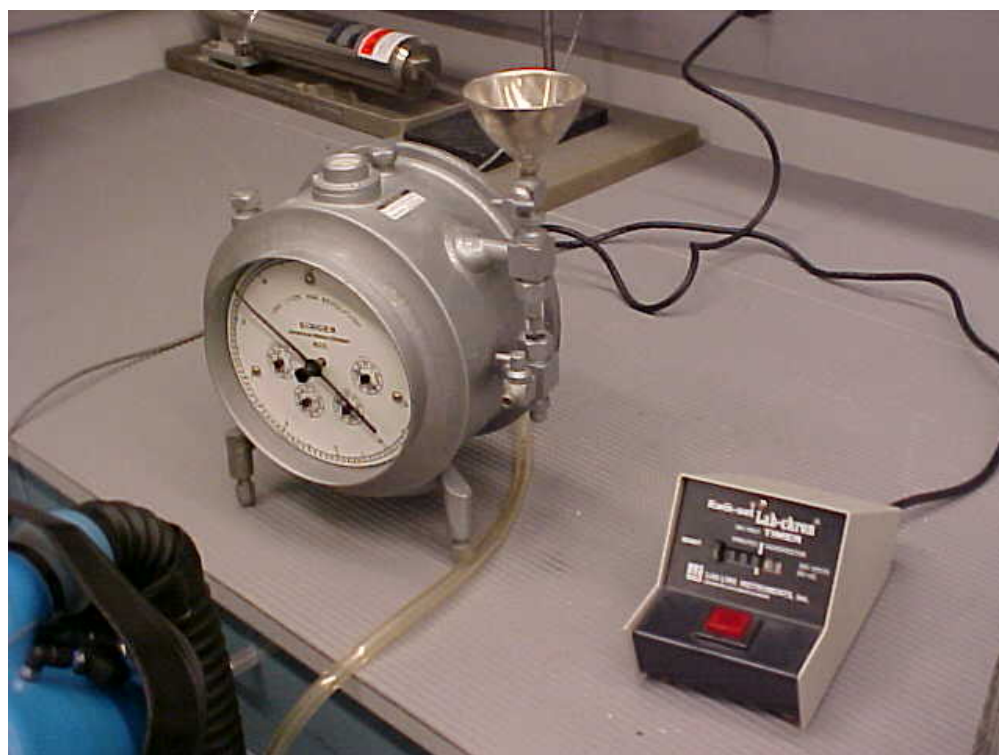

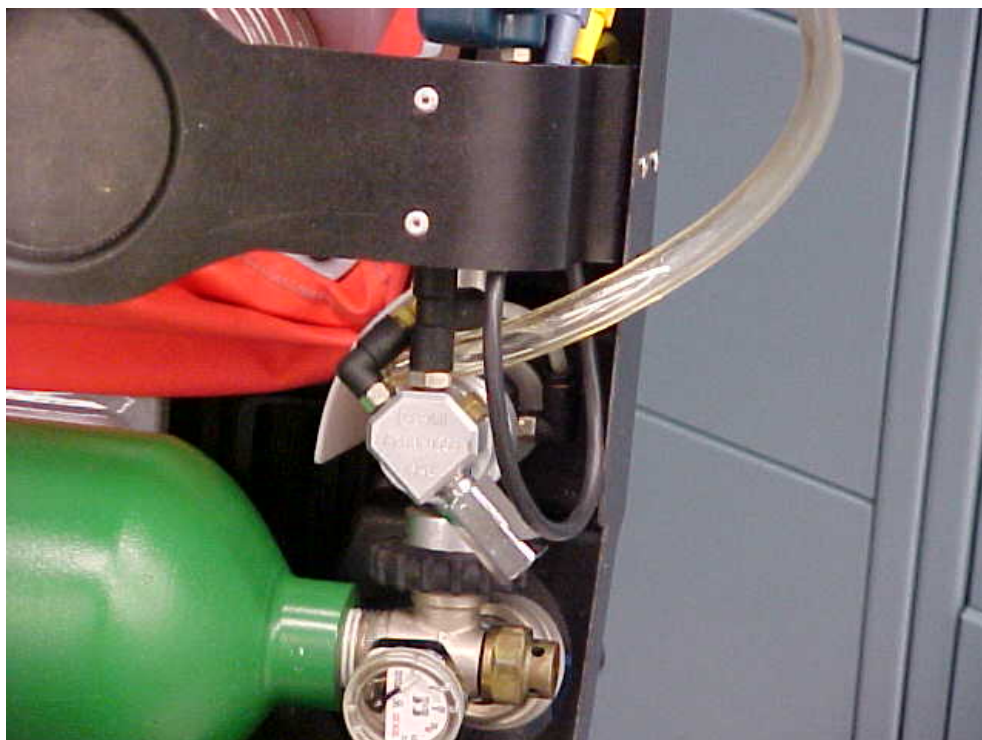

Revision History

Revision	Date	Reason for Revision
1.0	24 May 2001	Historic document
1.1	27 September 2005	Update header and format to reflect lab move from Morgantown, WV No changes to method