

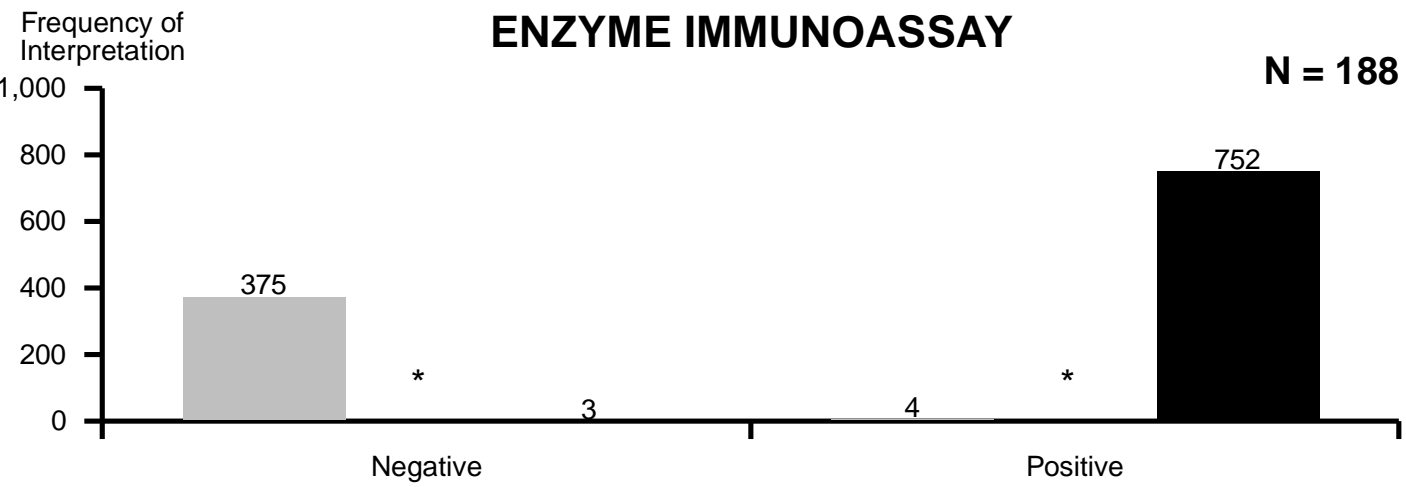



**Figure 1. Frequency of HTLV-I/II antibody test result interpretations, by sample type (reactivity), for the enzyme immunoassay (EIA), Western blot (WB), and indirect immunofluorescence (IIF), reported by participant laboratories for the May 20, 1996 shipment**

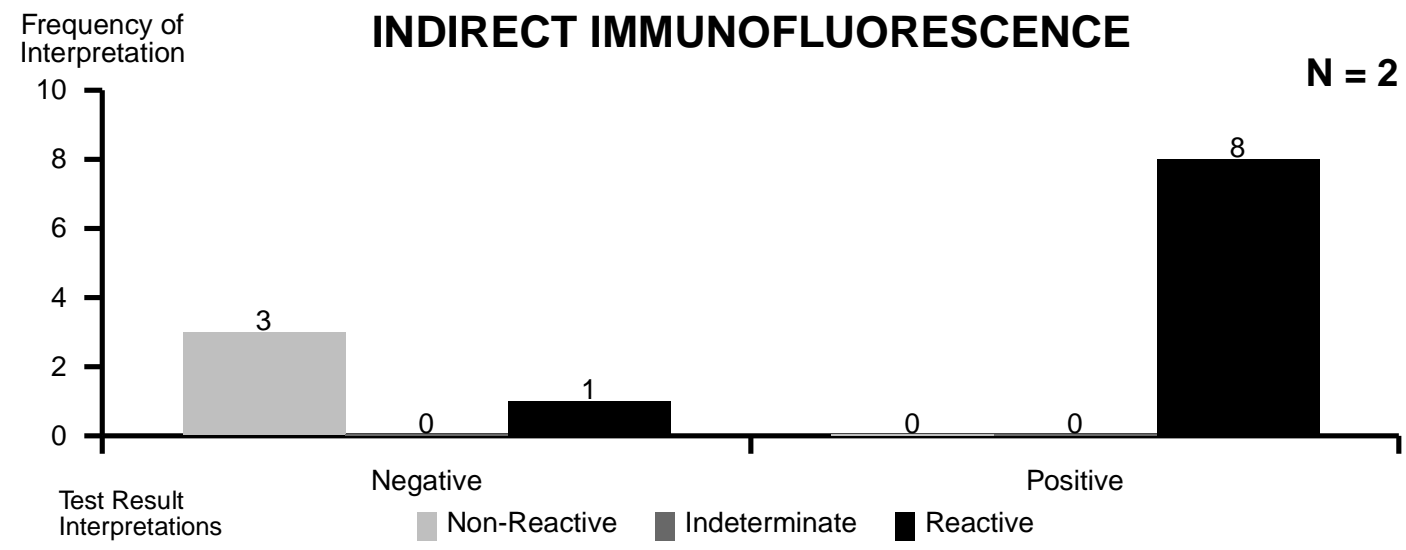


\* = Indeterminate is not an EIA interpretation option; these areas have been left blank

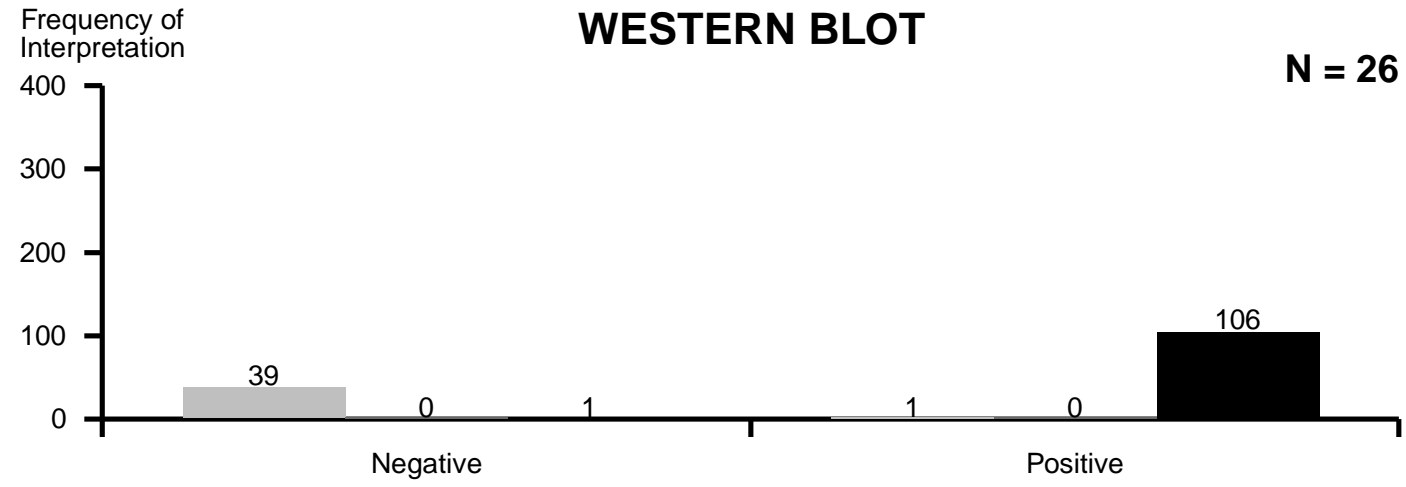




**Figure 2. Percentage of HTLV-I/II participant laboratories, by laboratory type, that reported results to the CDC for the May 20, 1996 shipment**

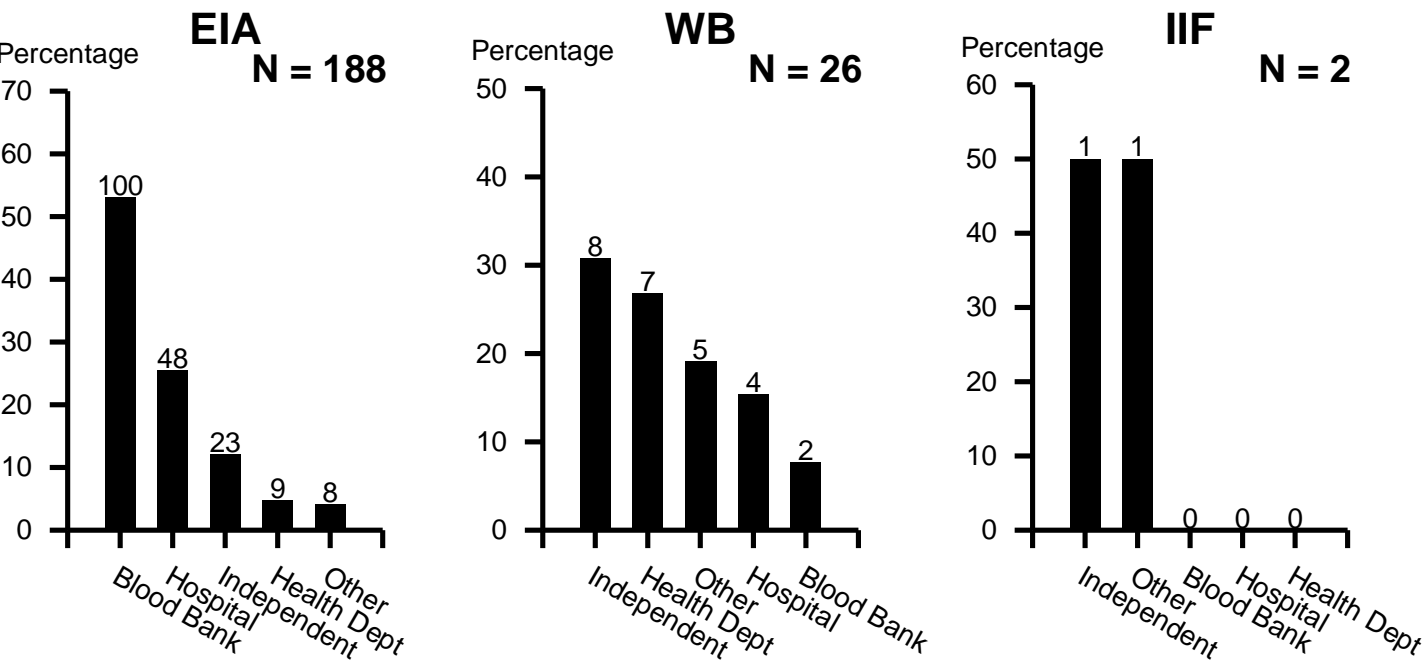



**Figure 3. Combination of HTLV-I/II tests reported by participant laboratories for the May 20, 1996 shipment**

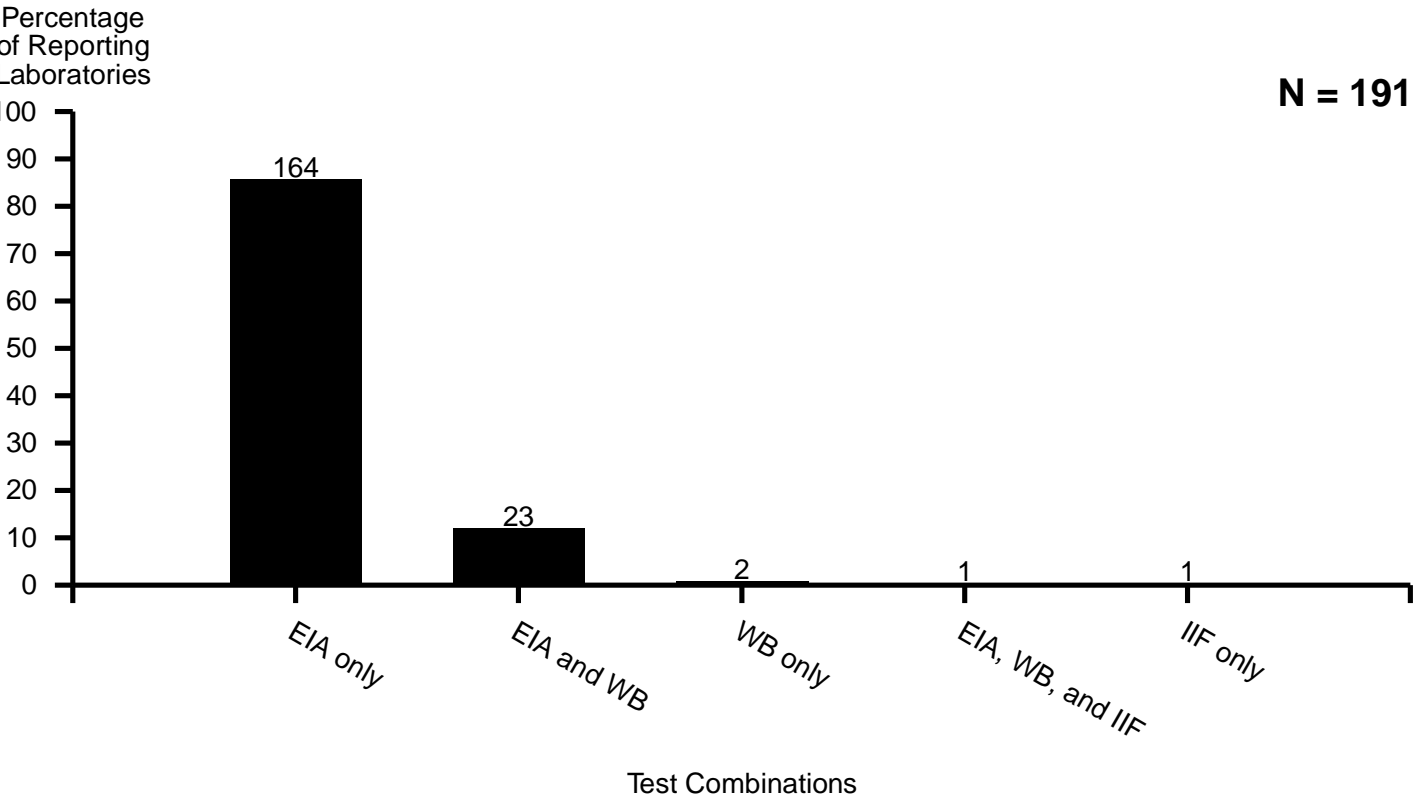

**Figure 4. Types of HTLV-I/II kits used for enzyme immunoassay, Western blot, and indirect immunofluorescence, as reported by participant laboratories to the CDC for the May 20, 1996 shipment**

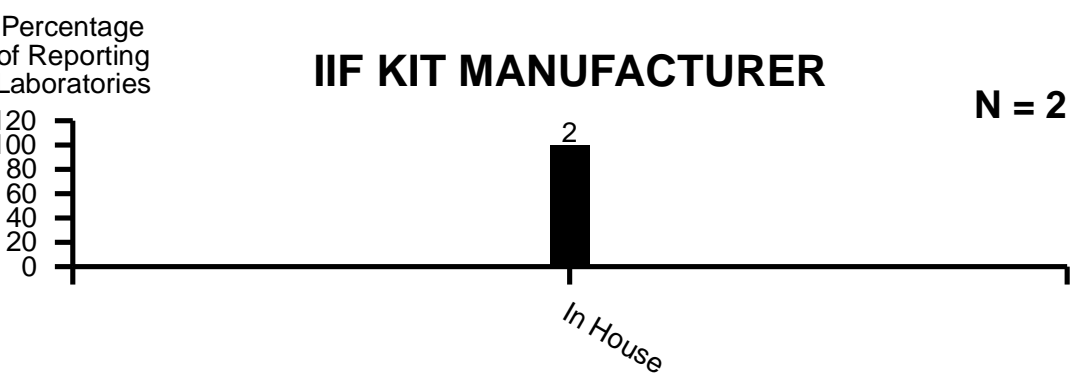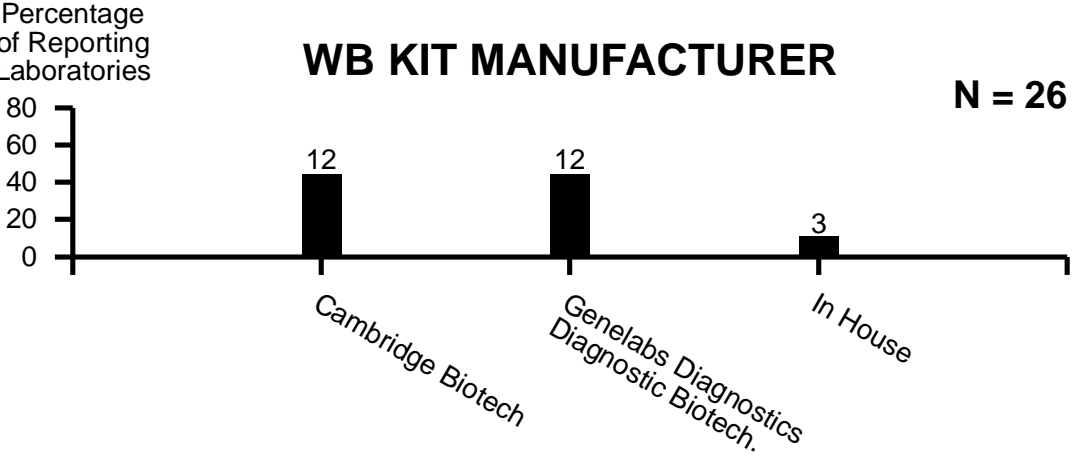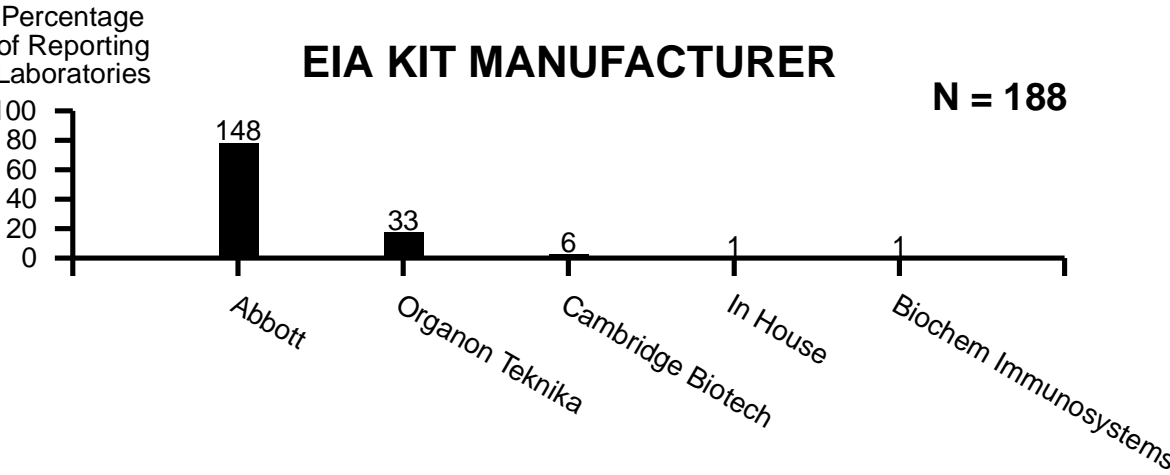



**Figure 5. Enzyme immunoassay HTLV-I/II results, by kit manufacturer, reported by participant laboratories for the May 20, 1996 shipment**

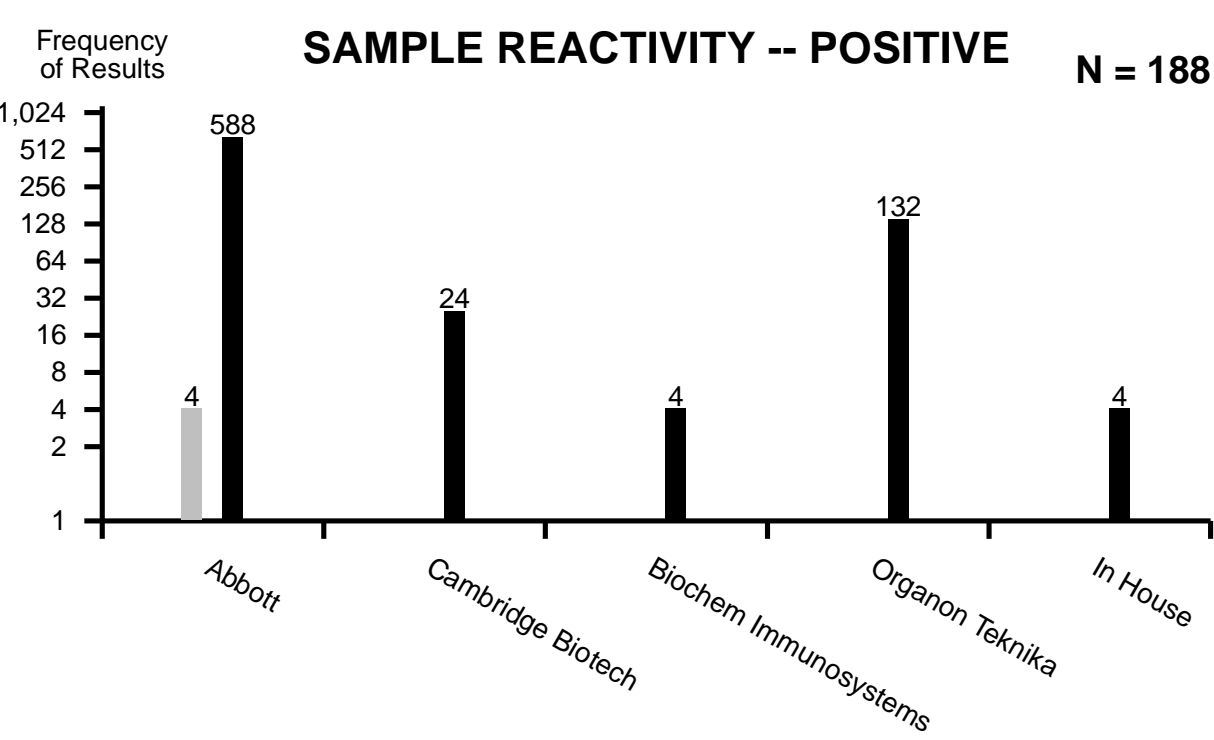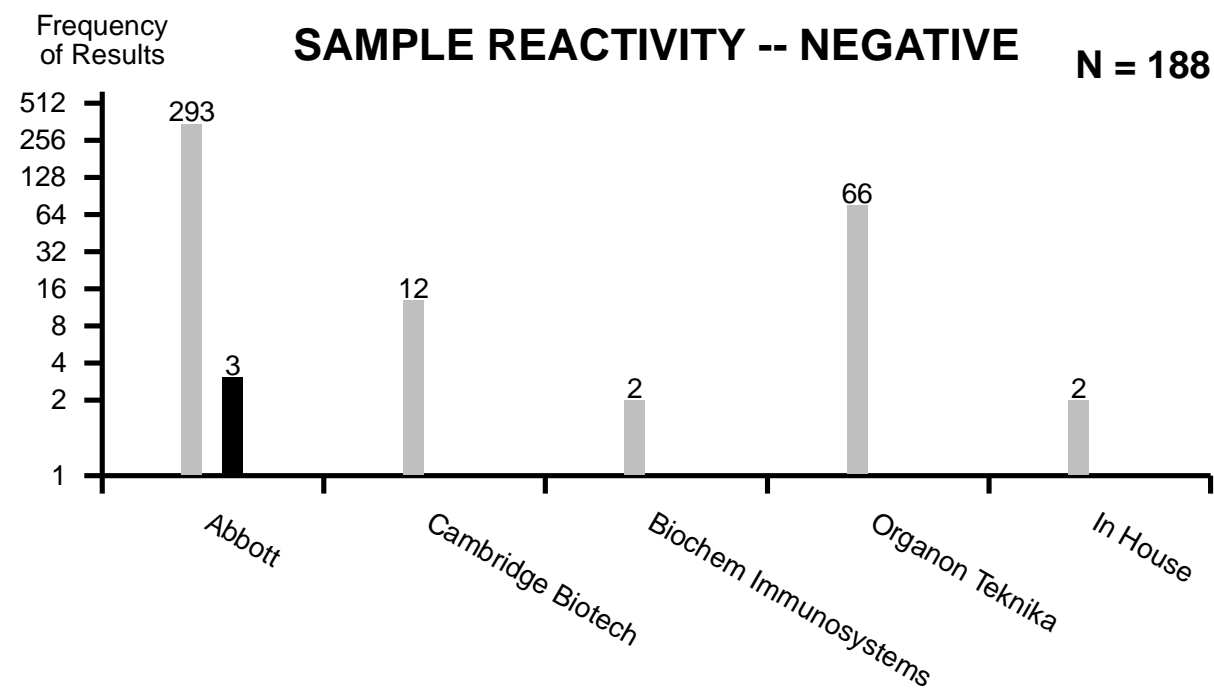

Test Result Interpretations

■ Non-Reactive    ■ Reactive


**Figure 6. Western blot HTLV-I/II results, by kit manufacturer, reported by participant laboratories for the May 20, 1996 shipment**

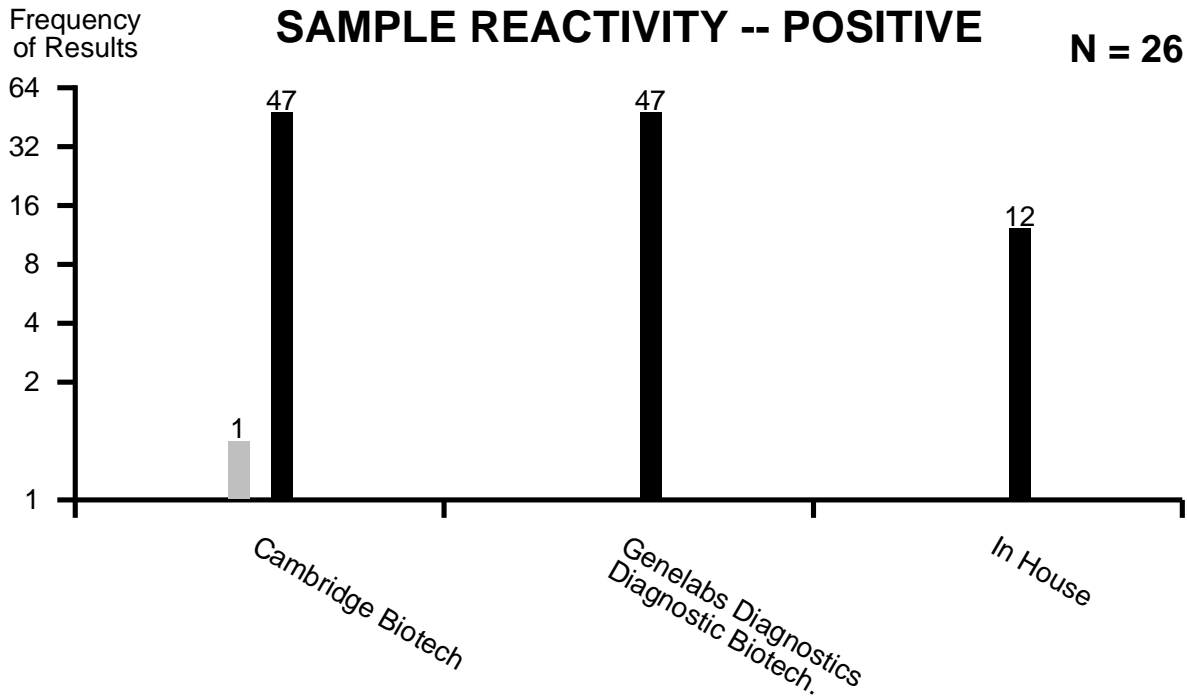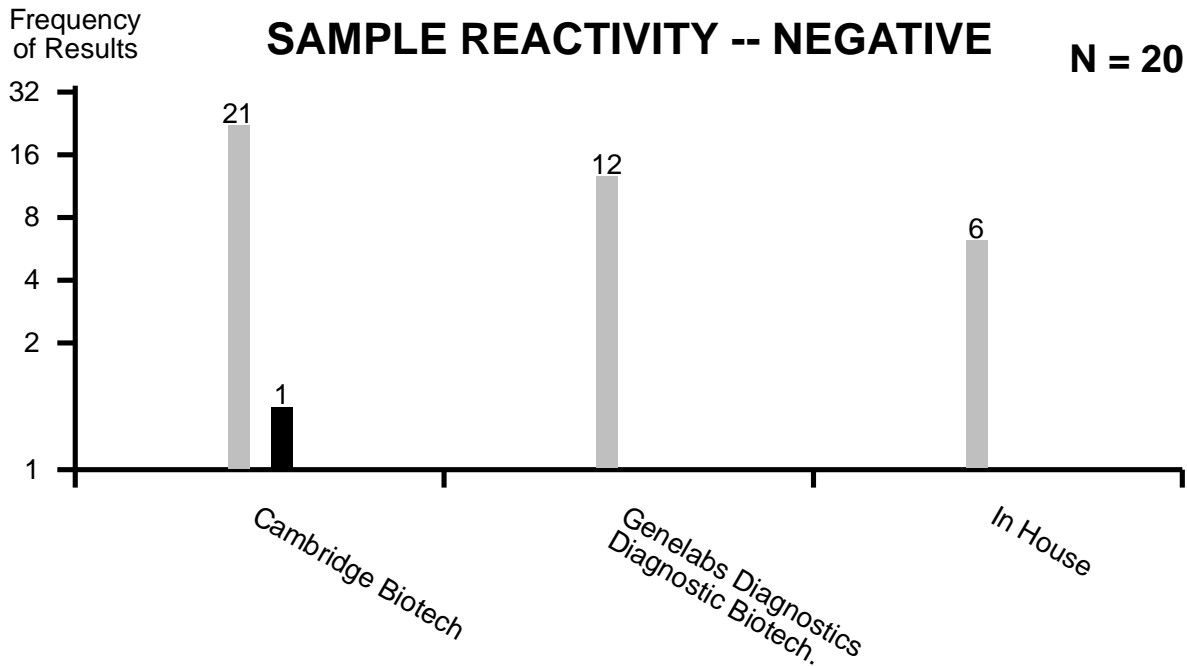


Test Result Interpretations: Non-Reactive (light gray), Indeterminate (medium gray), Reactive (black)

**Figure 7. Indirect immunofluorescence HTLV-I/II results, by kit manufacturer, reported by participant laboratories for the May 20, 1996 shipment**

**SAMPLE REACTIVITY -- NEGATIVE** **N = 2**

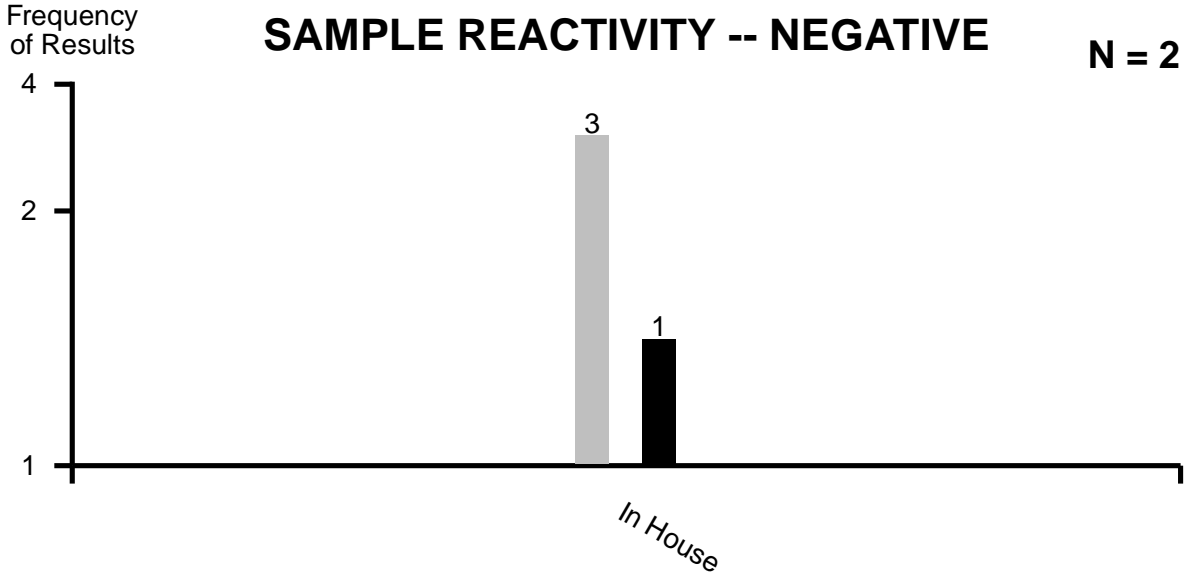


**SAMPLE REACTIVITY -- POSITIVE** **N = 2**

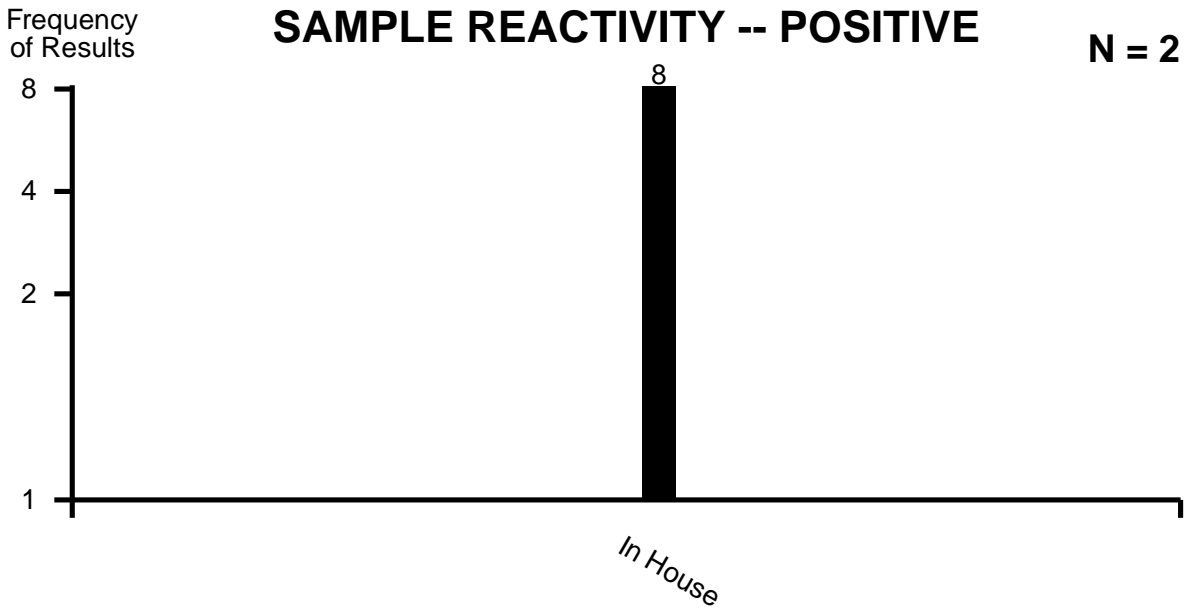


Test Result Interpretations      ■ Non-Reactive      ■ Indeterminate      ■ Reactive

**Figure 8. Western blot HTLV-I/II band patterns reported to CDC by participant laboratories for the May 20, 1996 shipment**

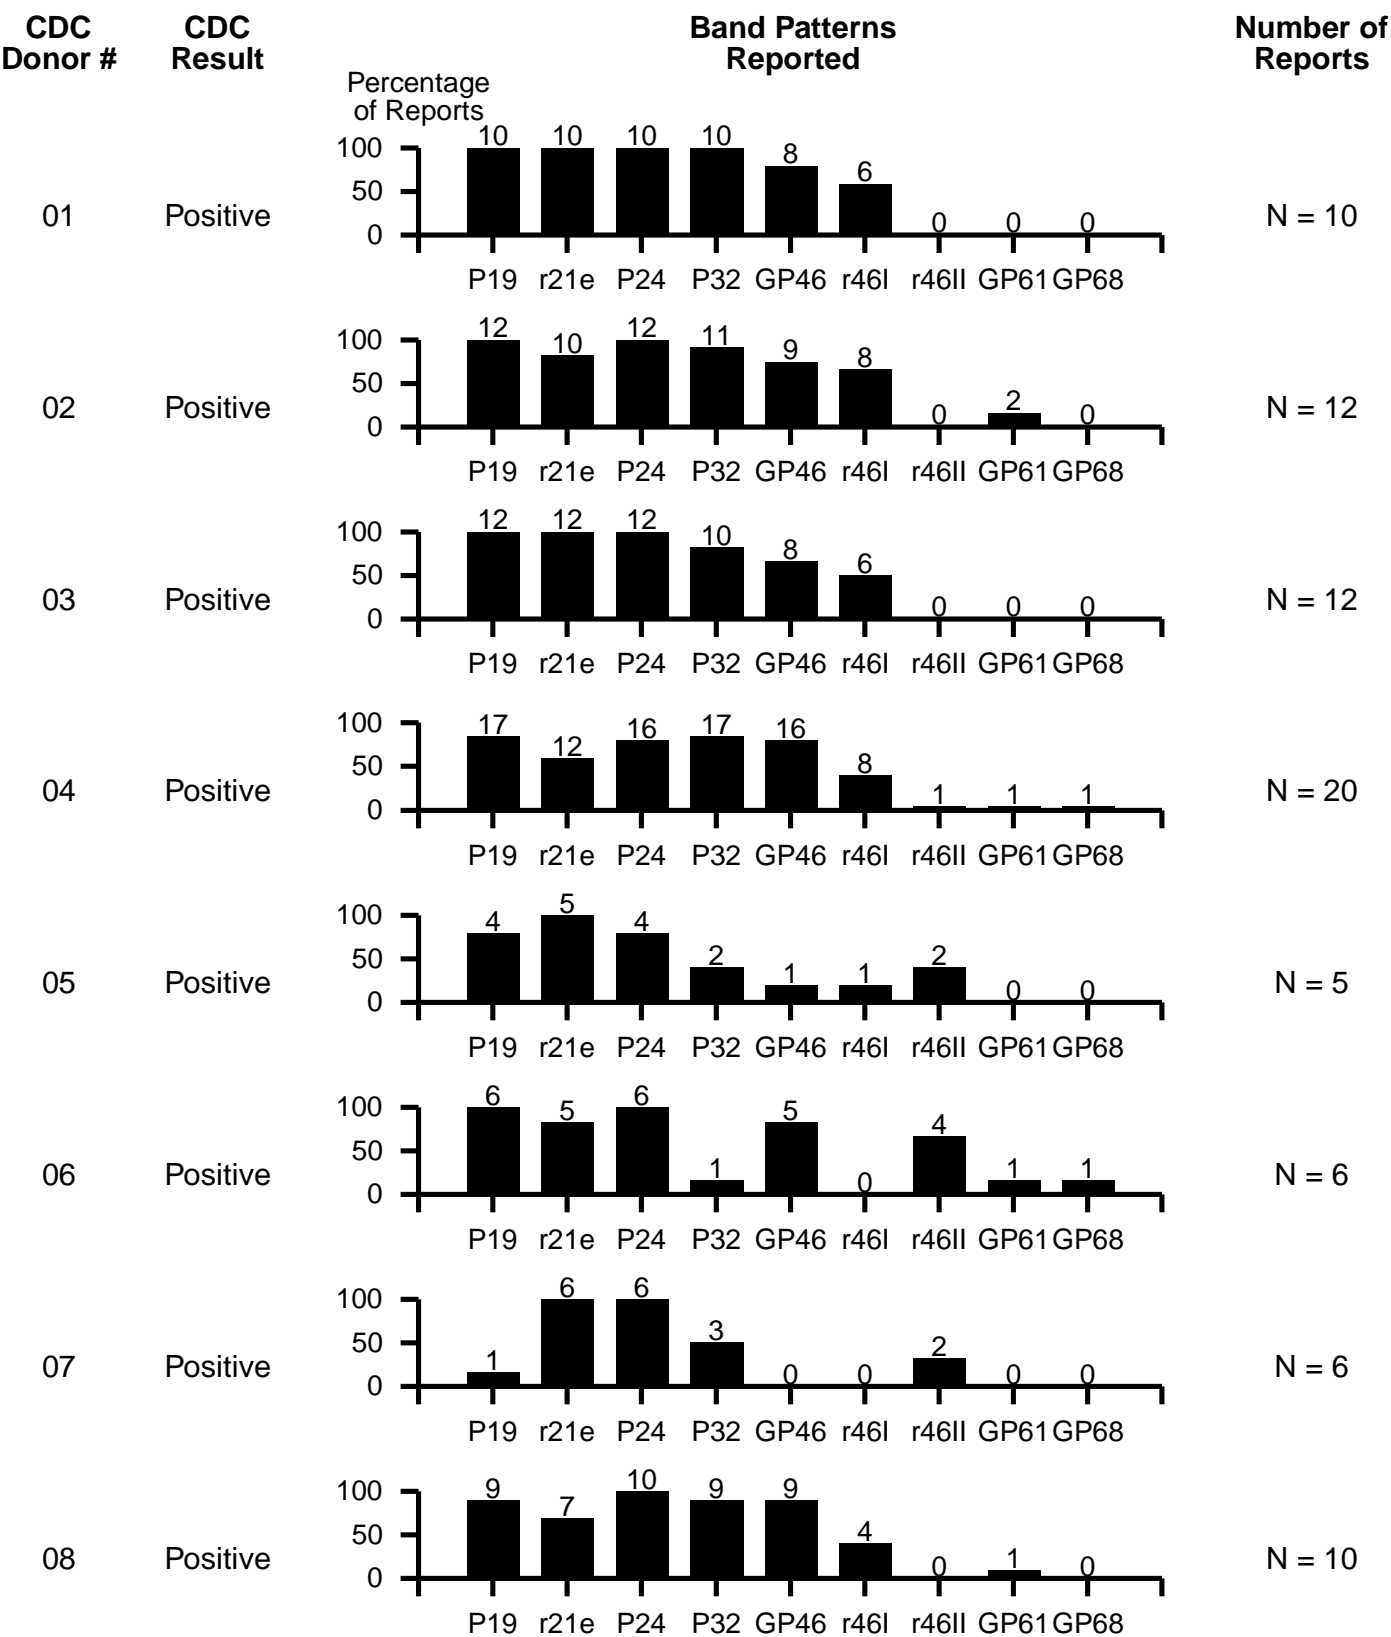


**Figure 8. Western blot HTLV-I/II band patterns reported to CDC by participant laboratories for the May 20, 1996 shipment**

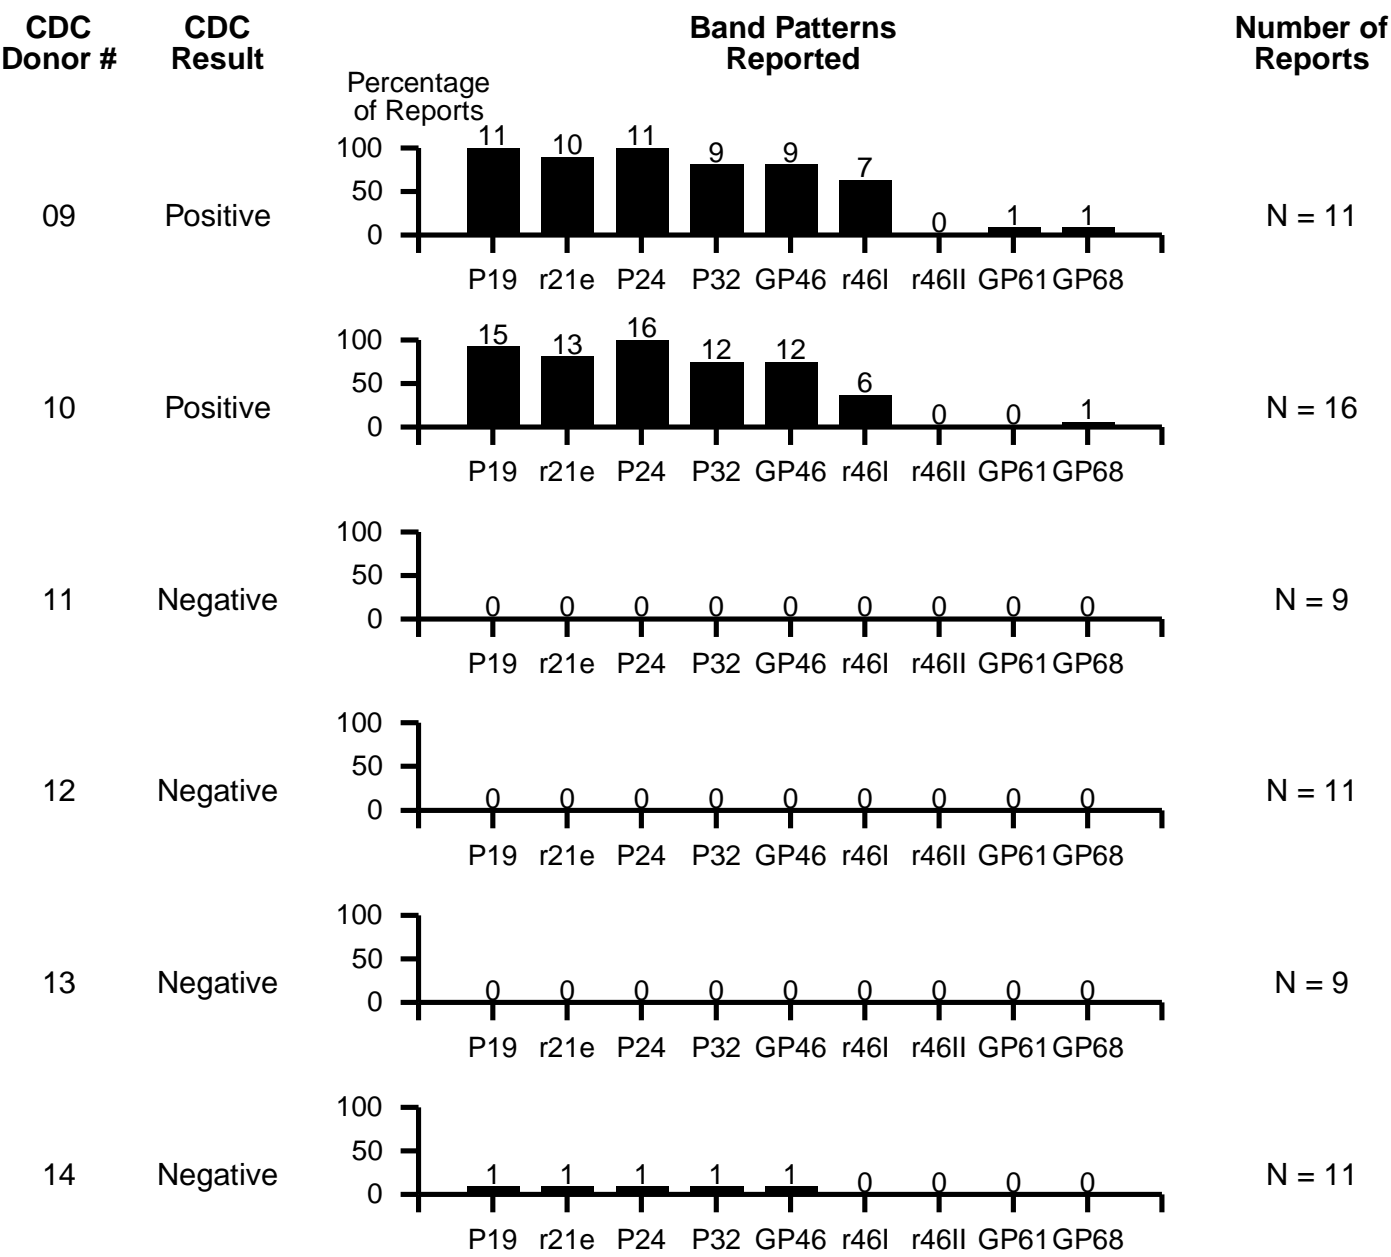







**Figure 9. Fluorescence intensity patterns, of HTLV-I/II-infected cells, for IIF results reported to CDC by participant laboratories for the May 20, 1996 shipment**

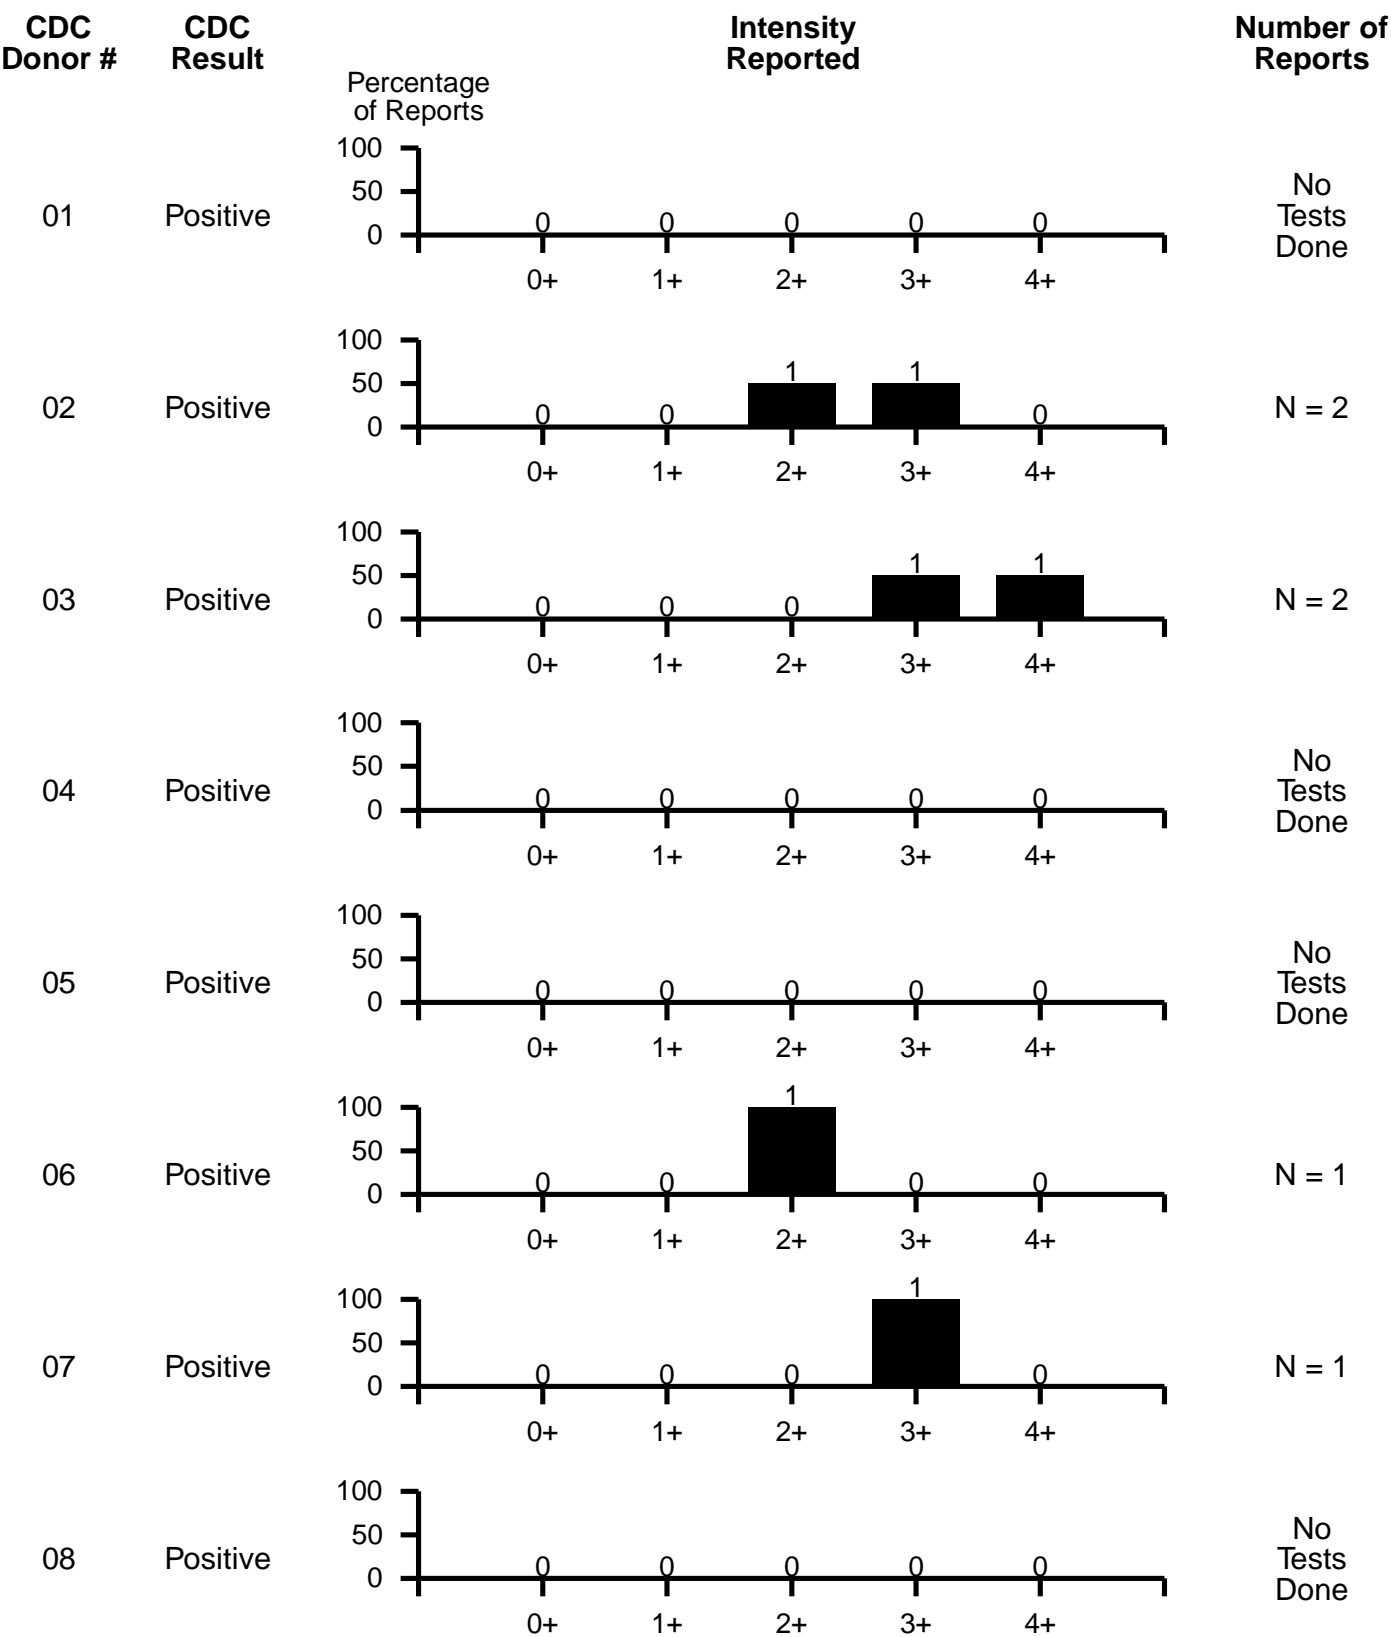

**Figure 9. Fluorescence intensity patterns, of HTLV-I/II-infected cells, for IIF results reported to CDC by participant laboratories for the May 20, 1996 shipment**

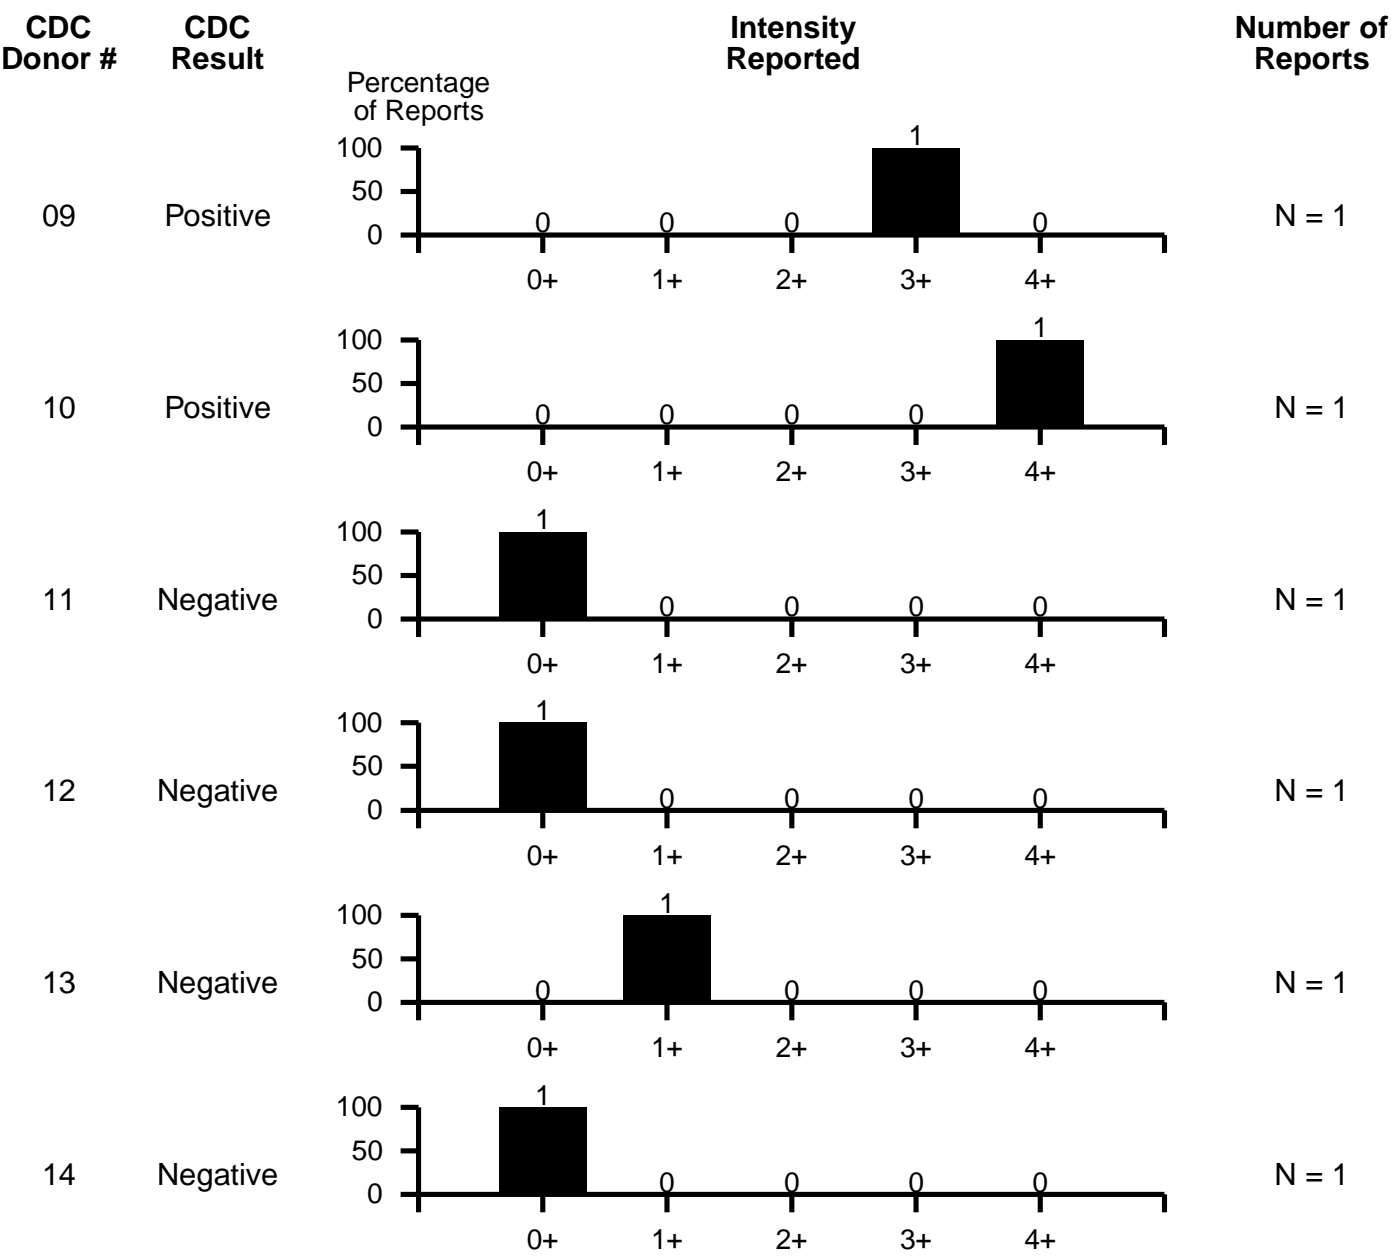

**Figure 10. Types of 'Other' HTLV test kits used and results reported by participant laboratories to the CDC for the May 20, 1996 shipment**

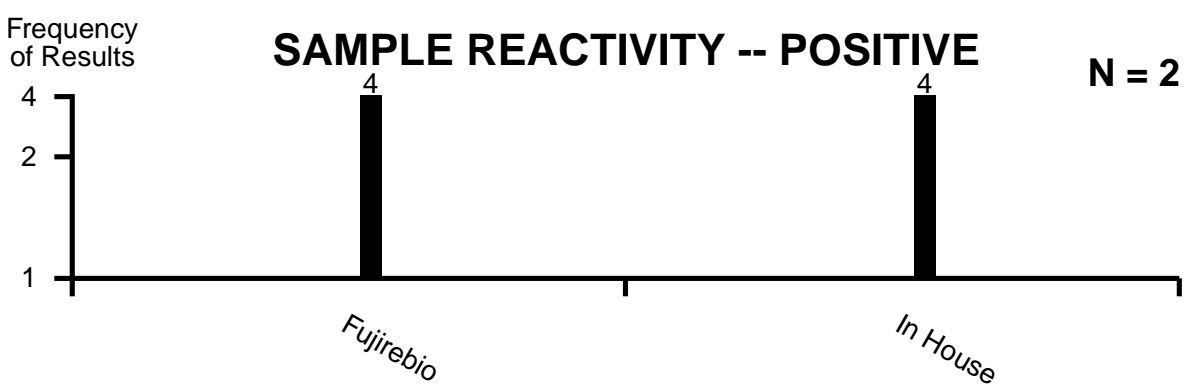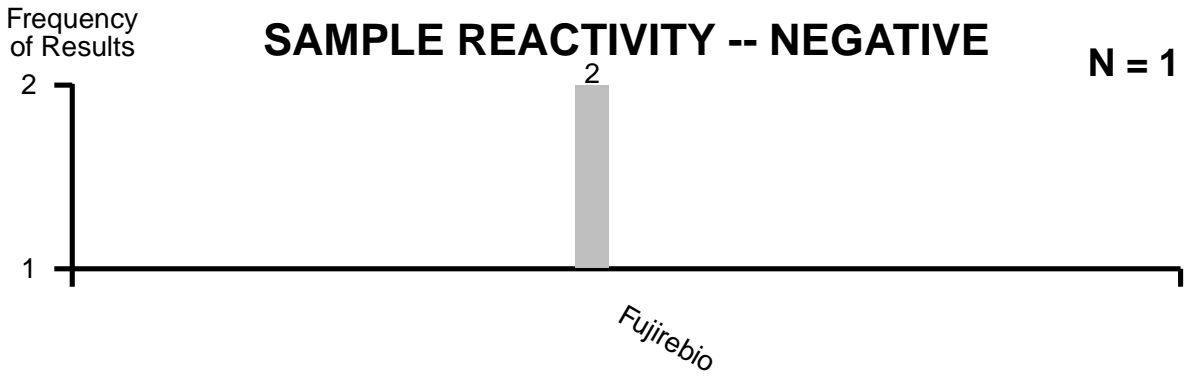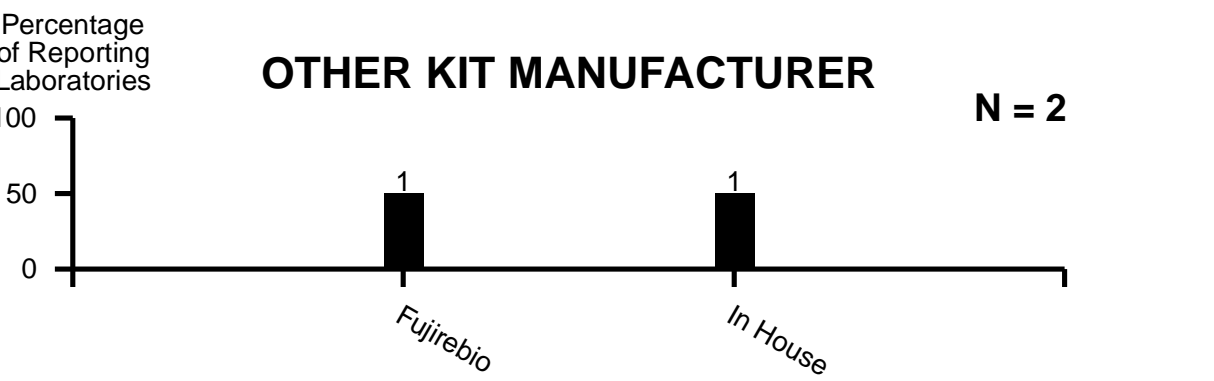

Test Result Interpretations

- Non-Reactive
- Indeterminate
- Reactive