


Figure 1. Frequency of HIV-1 antibody test result interpretations, by sample type (reactivity), for the enzyme immunoassay (EIA), Western blot (WB), and indirect immunofluorescence (IIF), reported by reference laboratories for the January 8, 1996 shipment

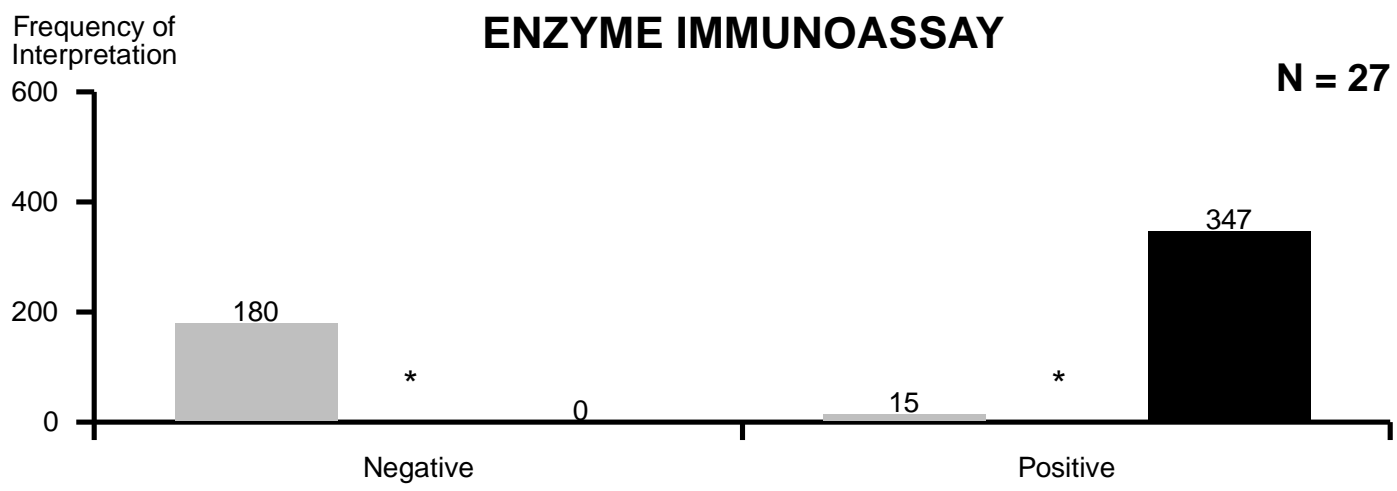

* = Indeterminate is not an EIA interpretation option; these areas have been left blank

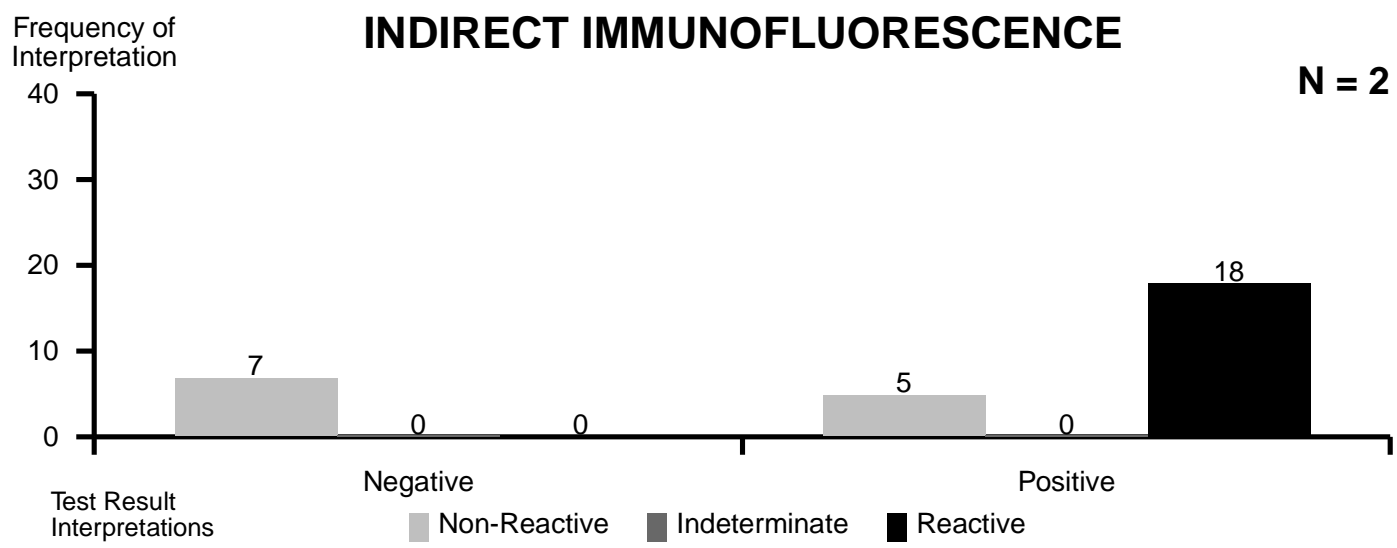
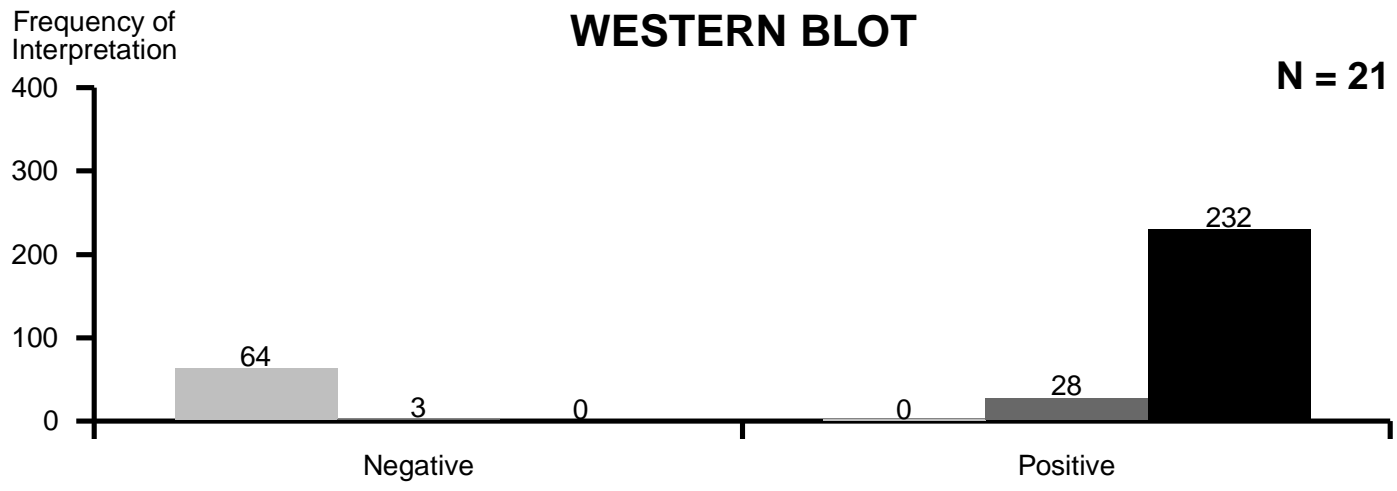


Figure 2. Percentage of HIV-1 reference laboratories, by laboratory type, that reported results to the CDC for the January 8, 1996 shipment

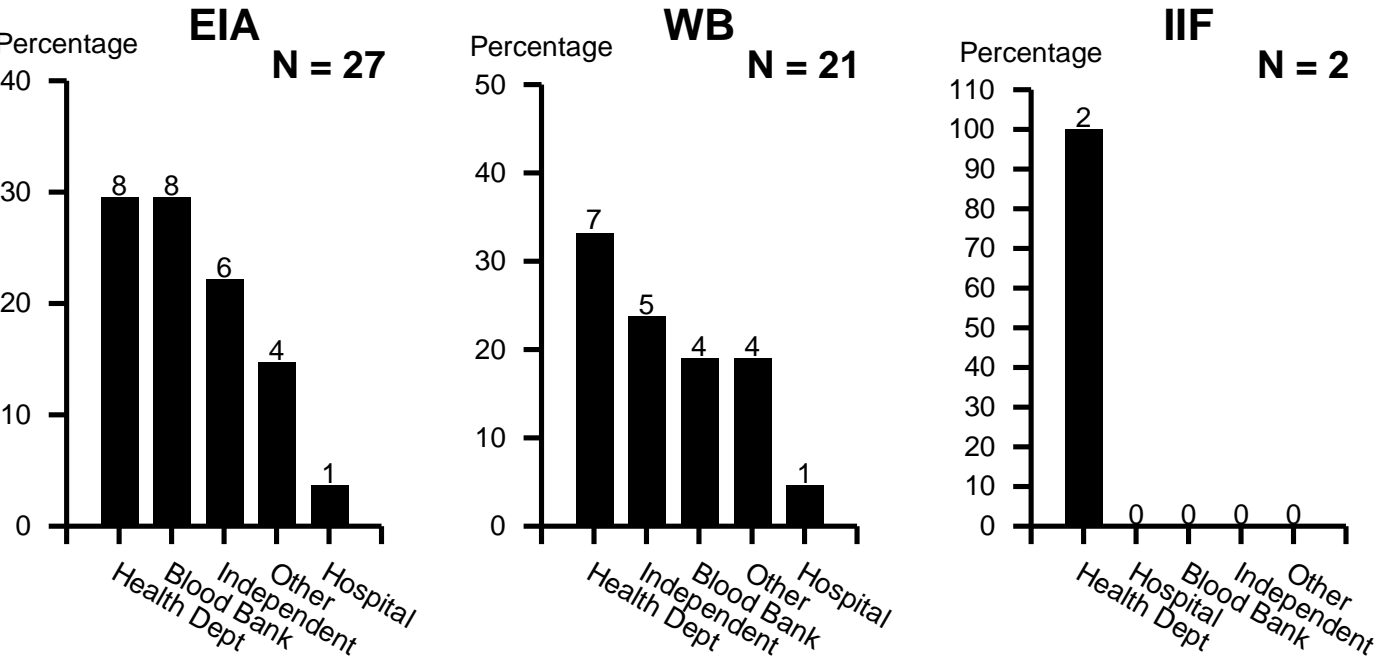


Figure 3. Combination of HIV-1 tests reported by reference laboratories for the January 8, 1996 shipment

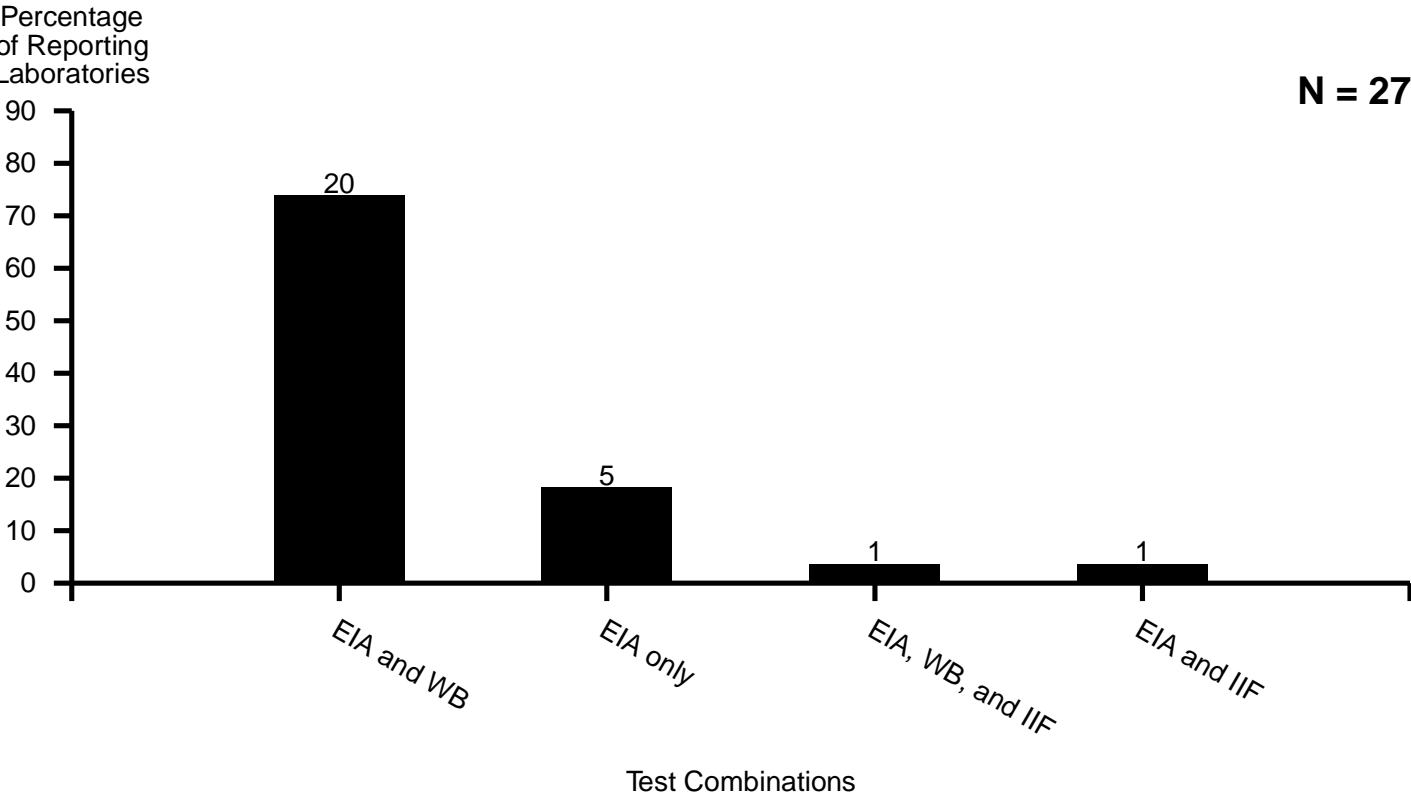


Figure 4. Types of HIV-1 kits used for enzyme immunoassay, Western blot, and indirect immunofluorescence, as reported by reference laboratories to the CDC for the January 8, 1996 shipment





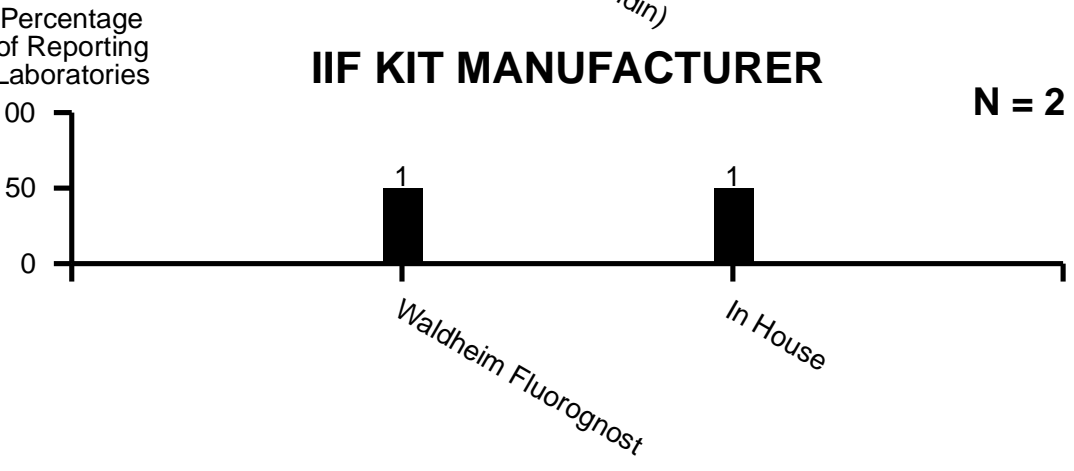




Figure 5. Enzyme immunoassay HIV-1 results, by kit manufacturer, reported by reference laboratories for the January 8, 1996 shipment

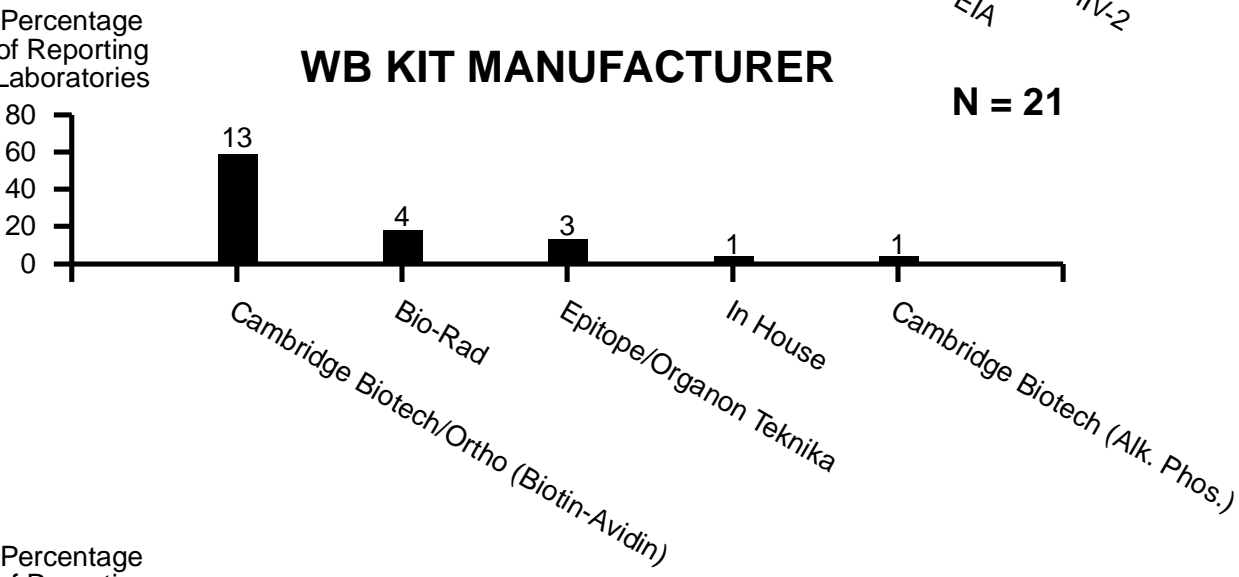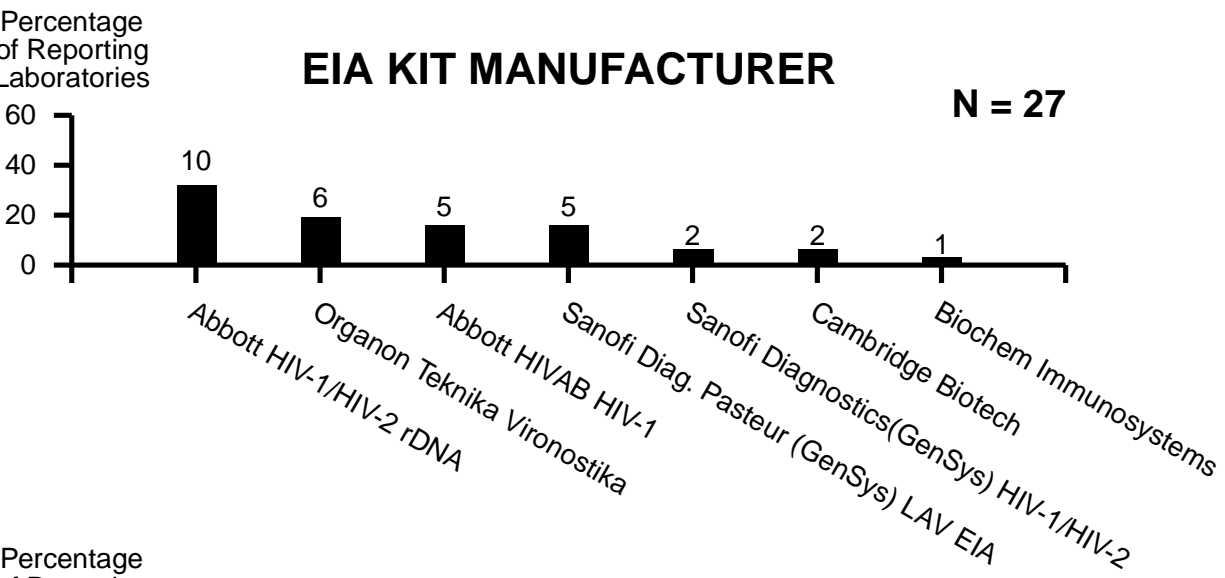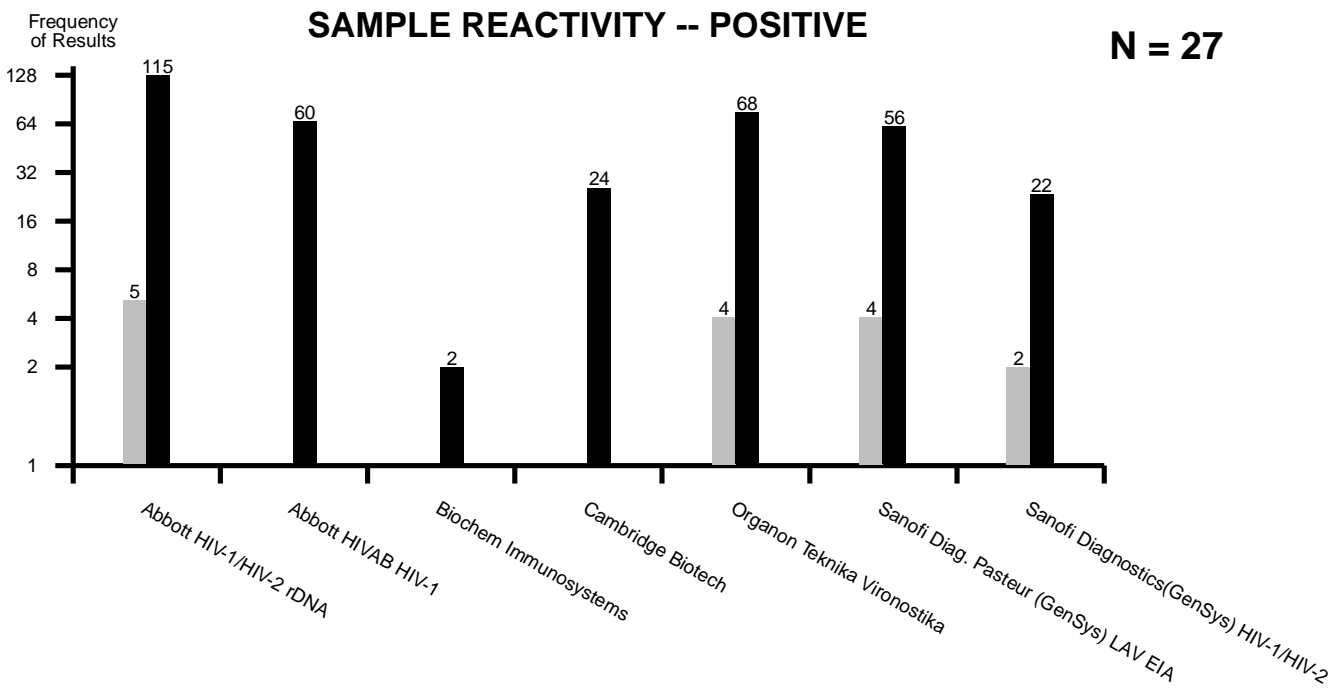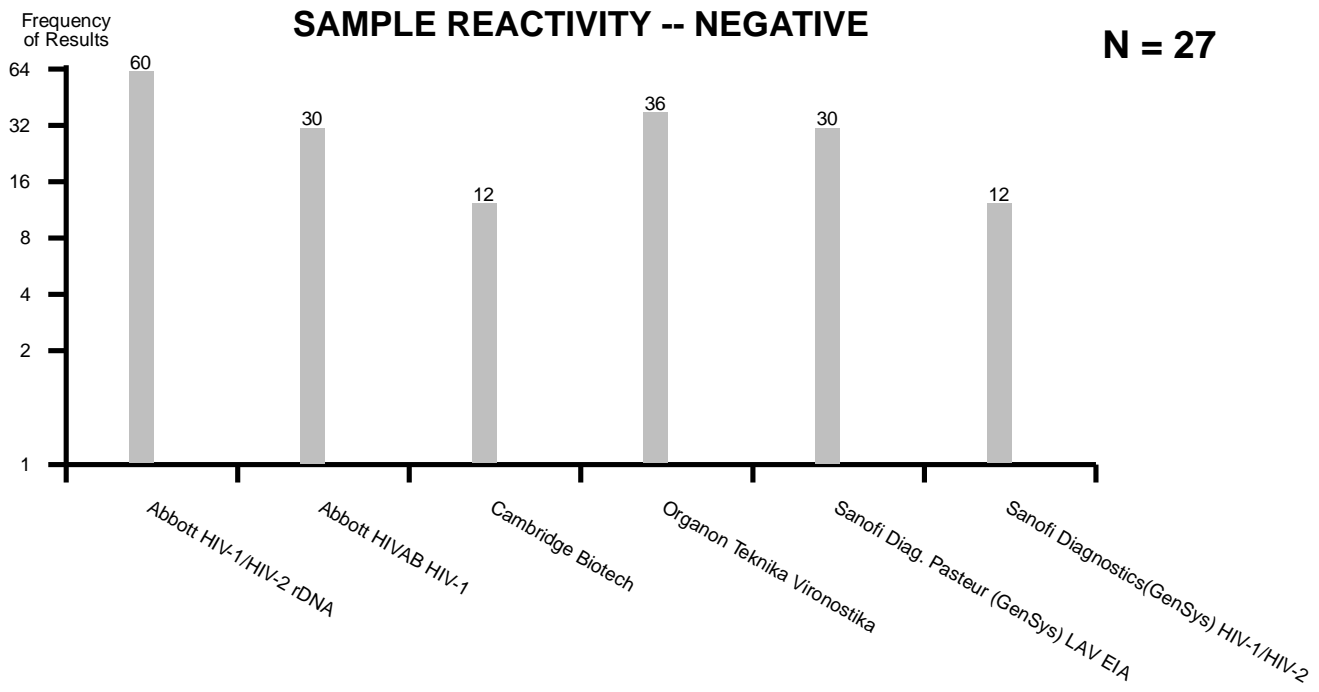

Test Result Interpretations

Non-Reactive
 Reactive



Figure 6. Western blot HIV-1 results, by kit manufacturer, reported by reference laboratories for the January 8, 1996 shipment

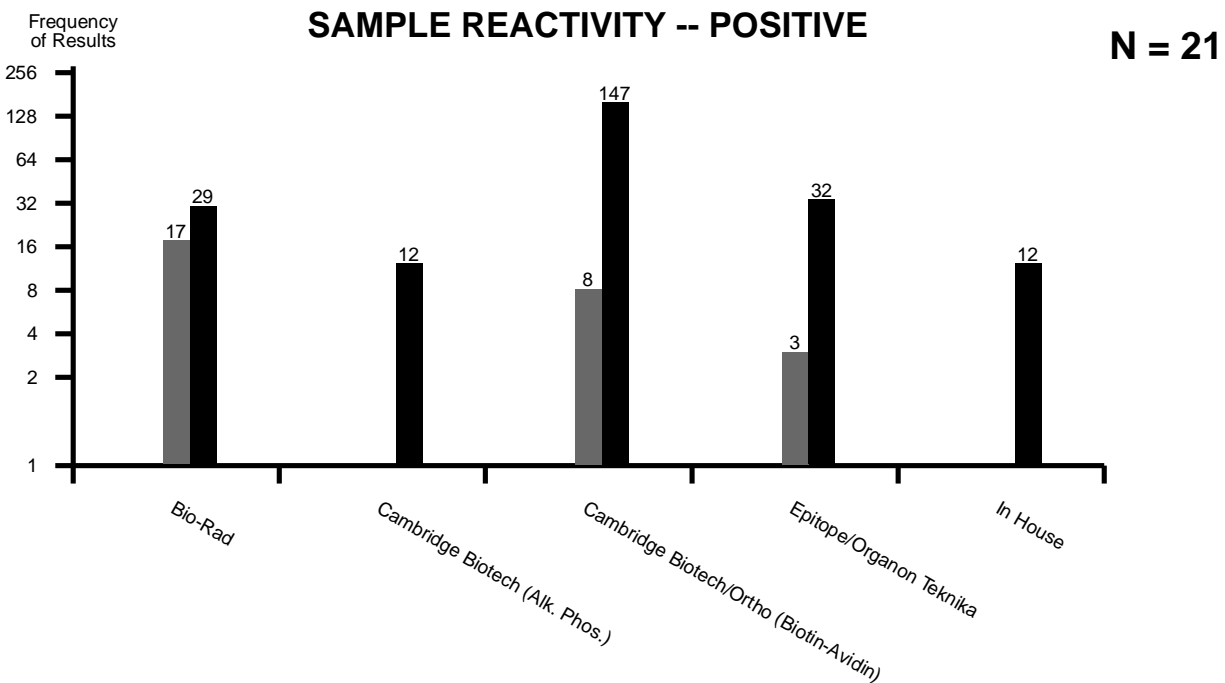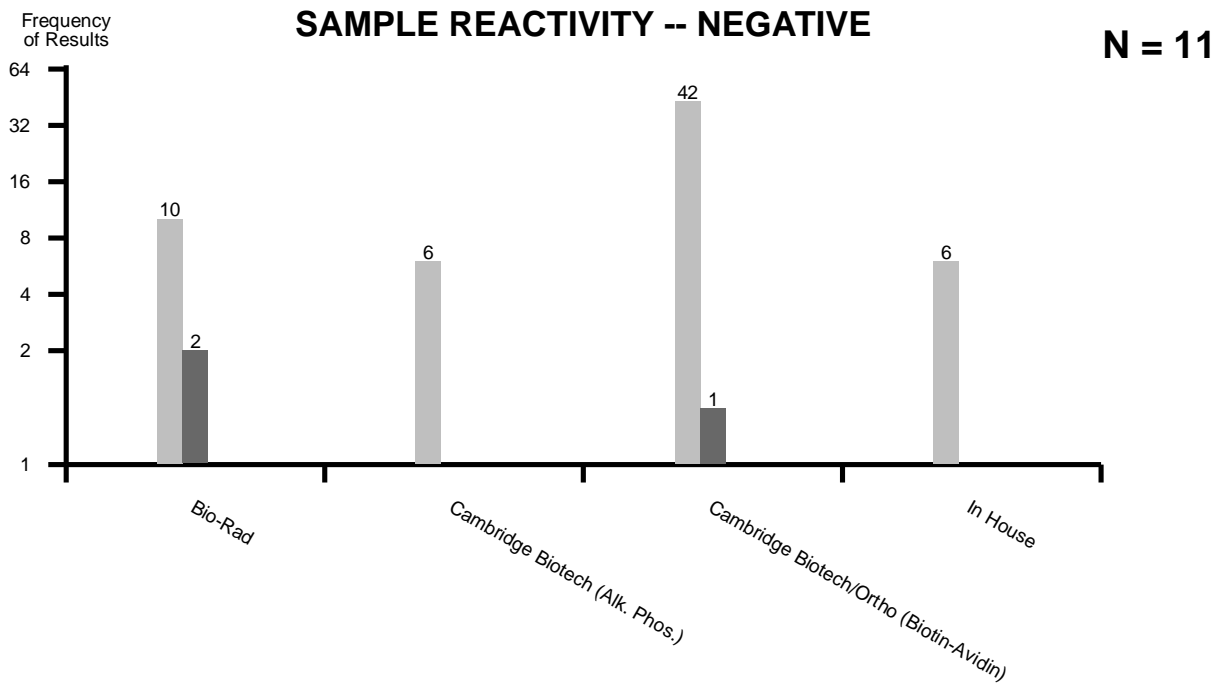

Test Result Interpretations

Non-Reactive
 Indeterminate
 Reactive

Figure 7. Indirect immunofluorescence HIV-1 results, by kit manufacturer, reported by reference laboratories for the January 8, 1996 shipment

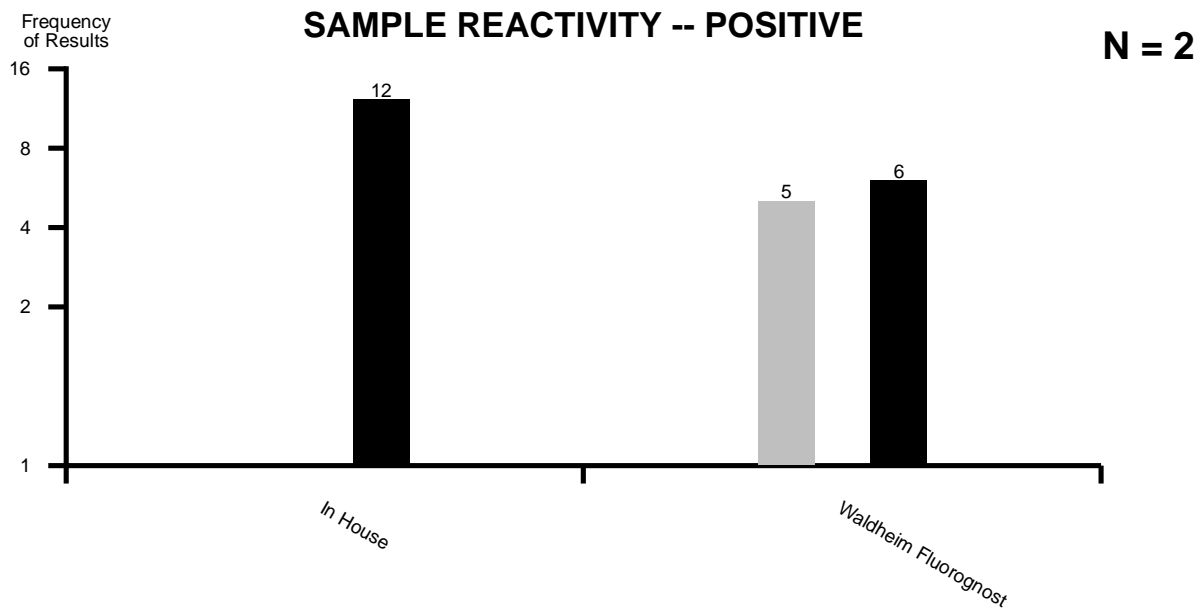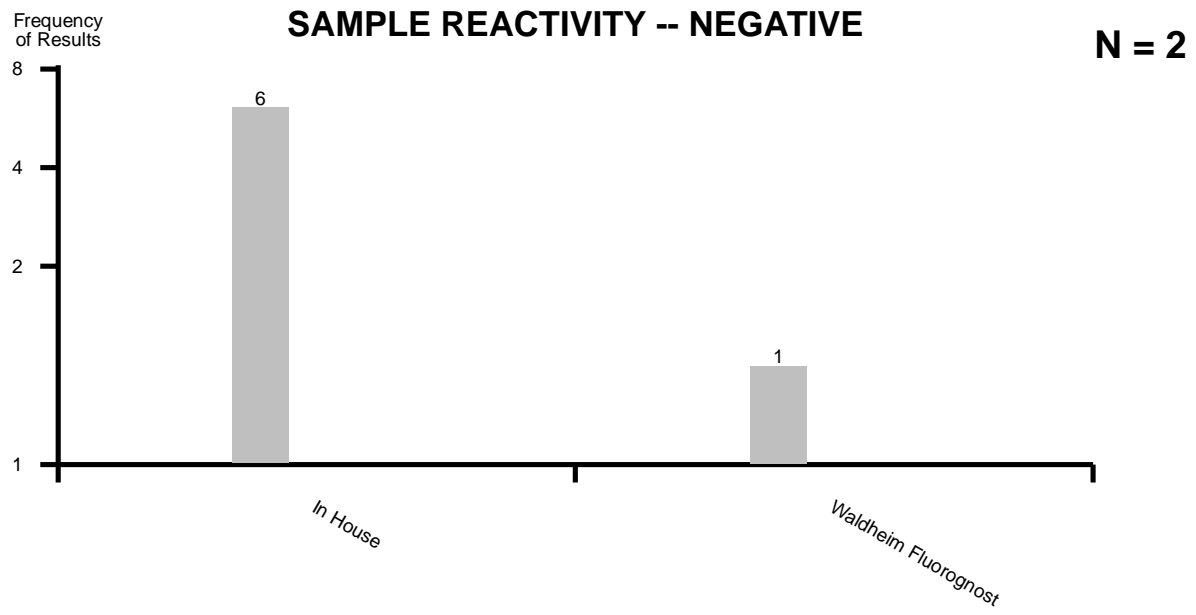

Test Result Interpretations

Non-Reactive
 Indeterminate
 Reactive

Figure 8. Western blot HIV-1 band patterns reported to CDC by reference laboratories for the January 8, 1996 shipment

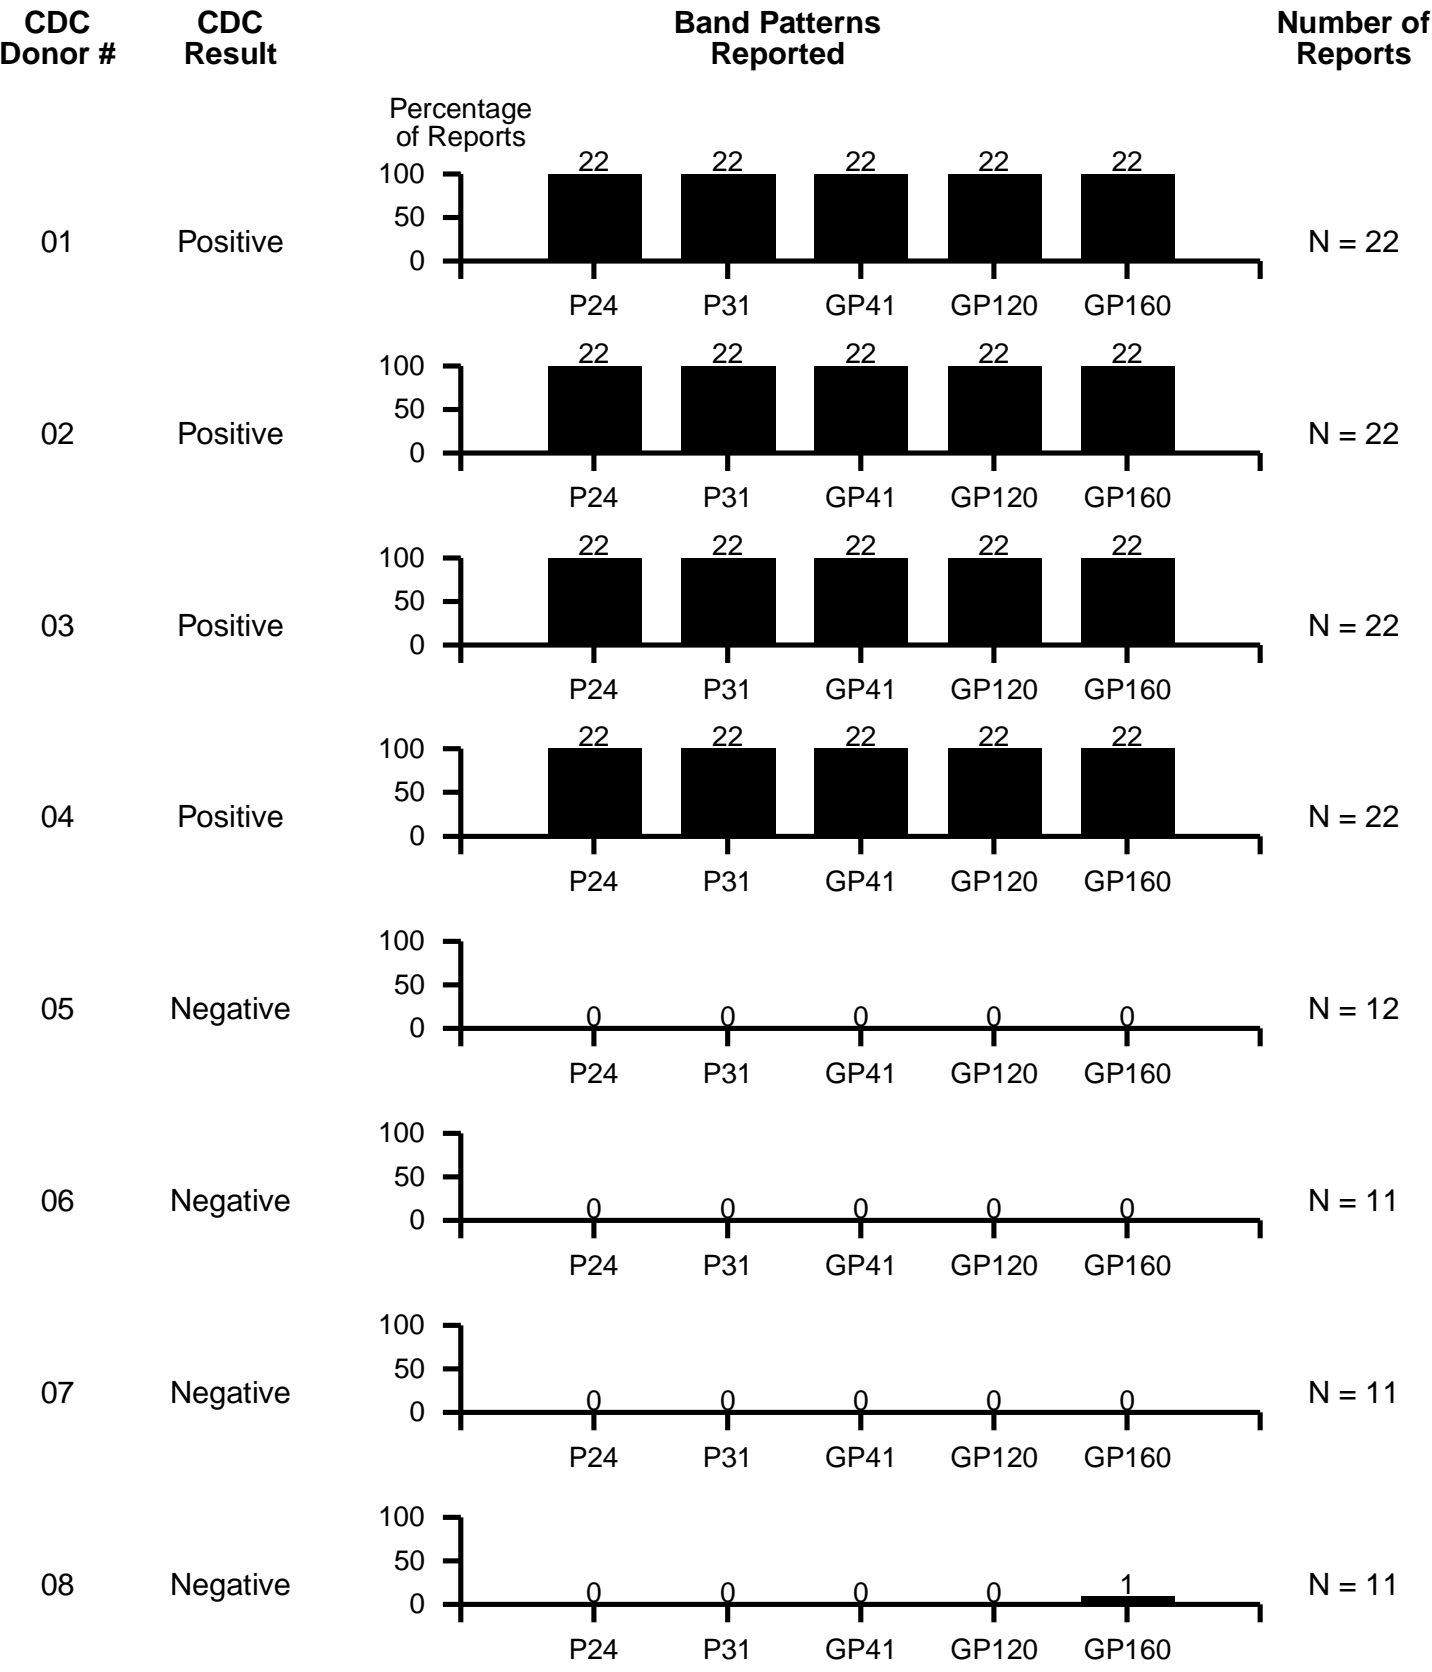


Figure 8. Western blot HIV-1 band patterns reported to CDC by reference laboratories for the January 8, 1996 shipment

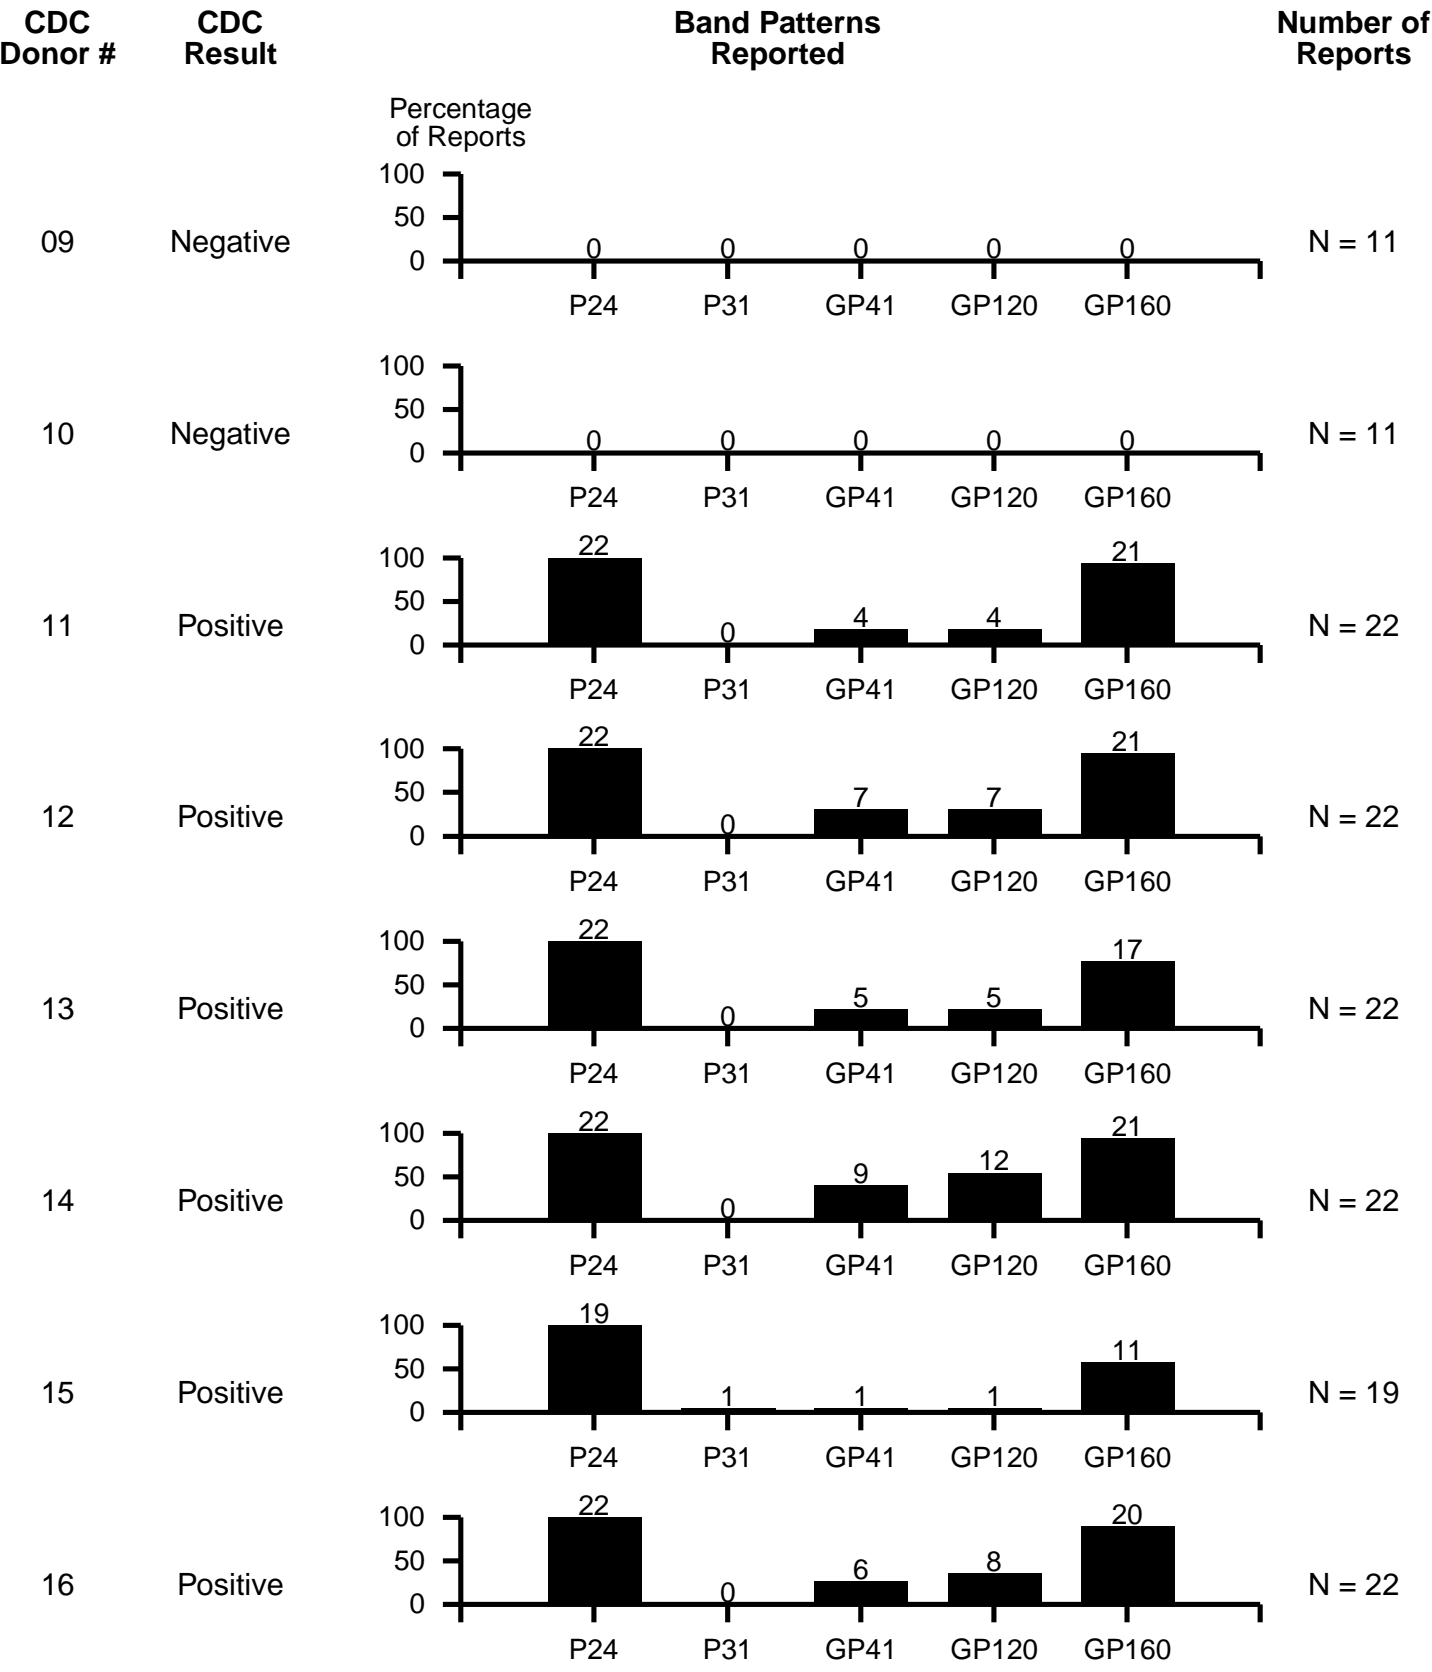


Figure 8. Western blot HIV-1 band patterns reported to CDC by reference laboratories for the January 8, 1996 shipment

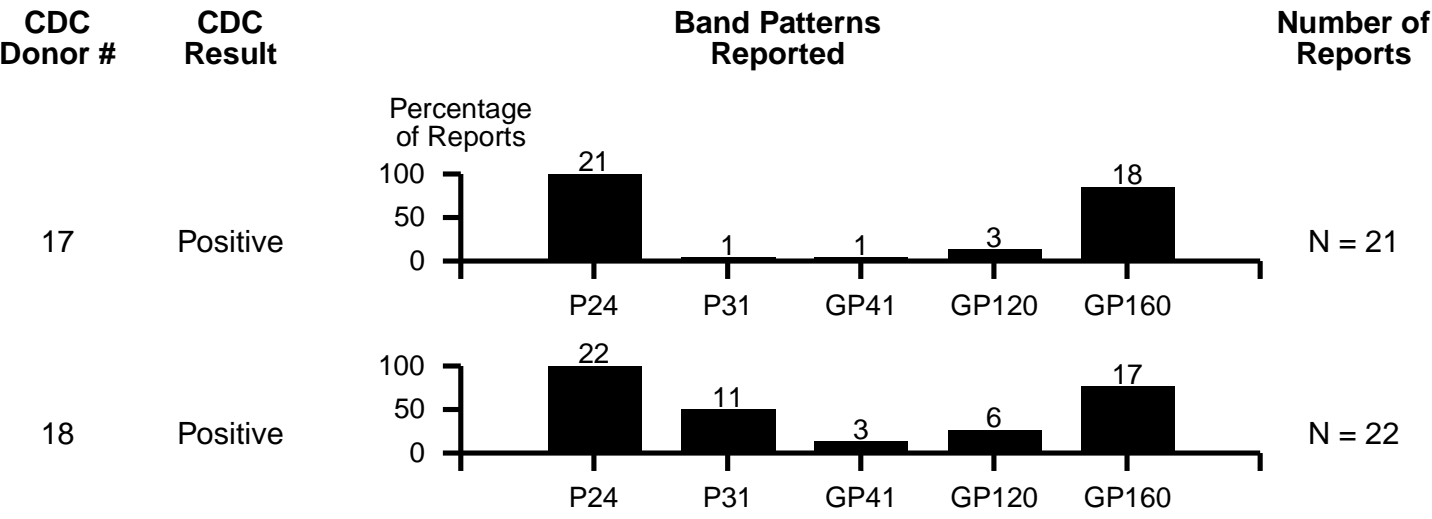


Figure 9. Fluorescence intensity patterns, of HIV-1-infected cells, for IIF results reported to CDC by reference laboratories for the January 8, 1996 shipment

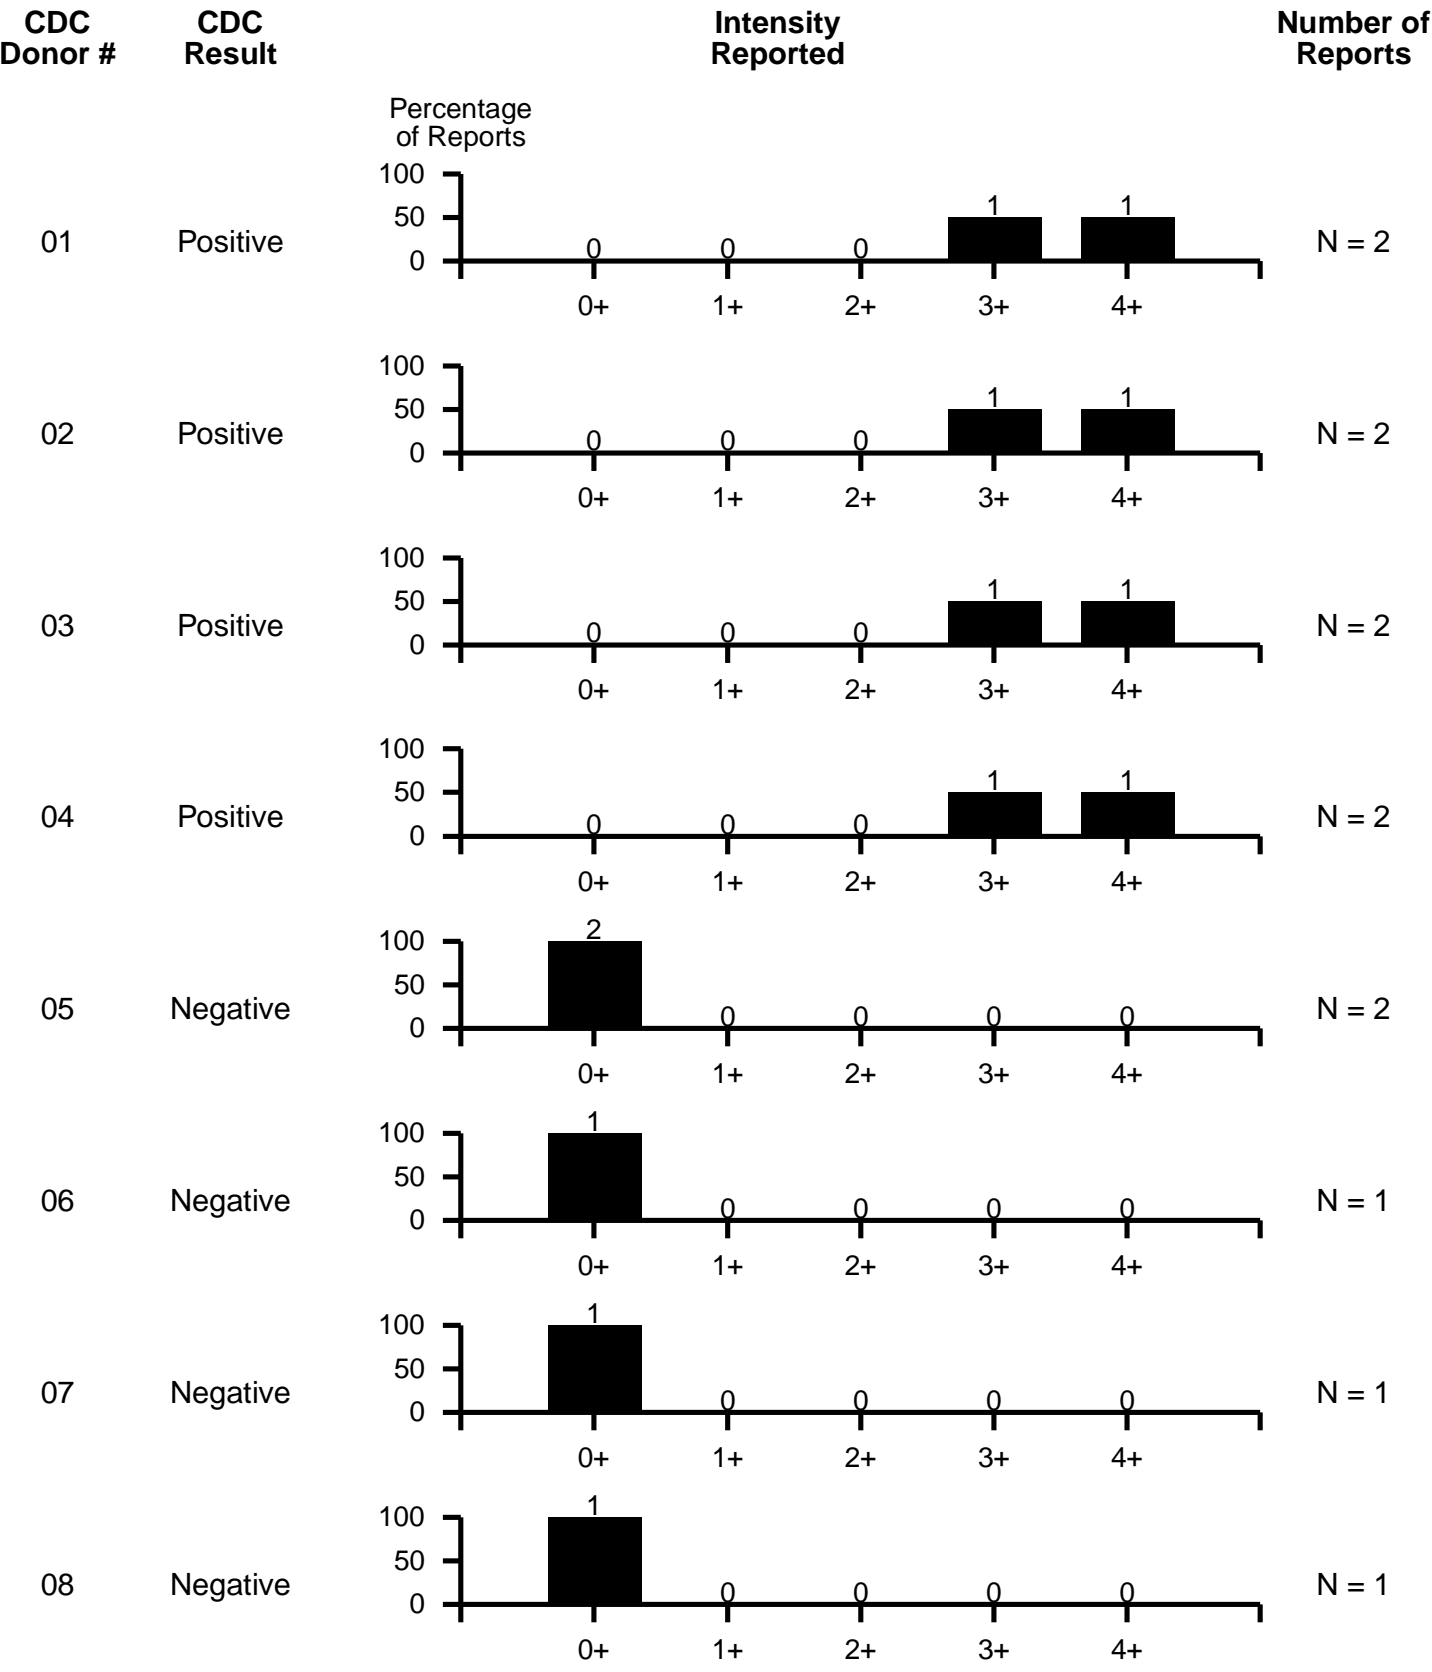


Figure 9. Fluorescence intensity patterns, of HIV-1-infected cells, for IIF results reported to CDC by reference laboratories for the January 8, 1996 shipment

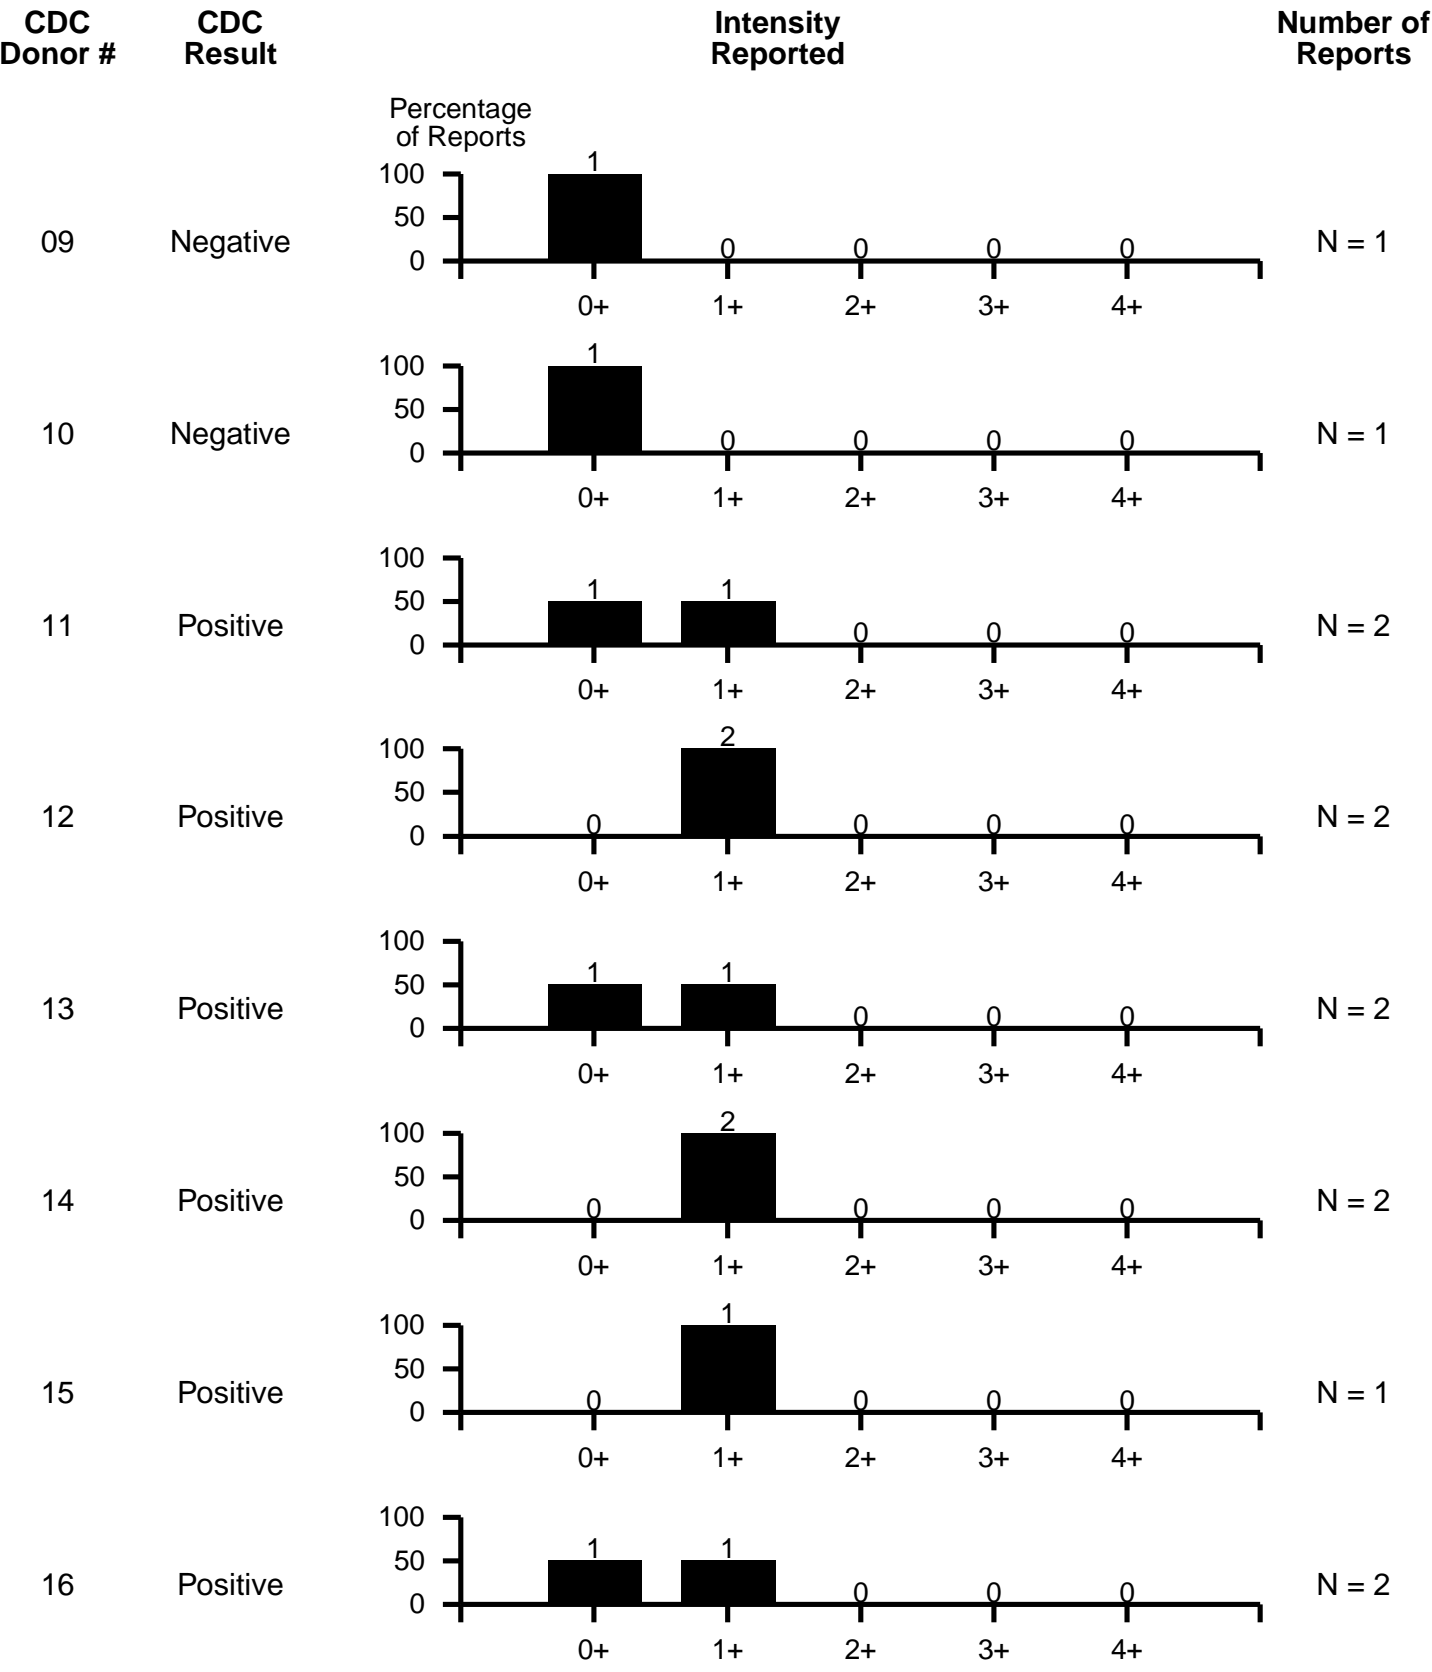


Figure 9. Fluorescence intensity patterns, of HIV-1-infected cells, for IIF results reported to CDC by reference laboratories for the January 8, 1996 shipment

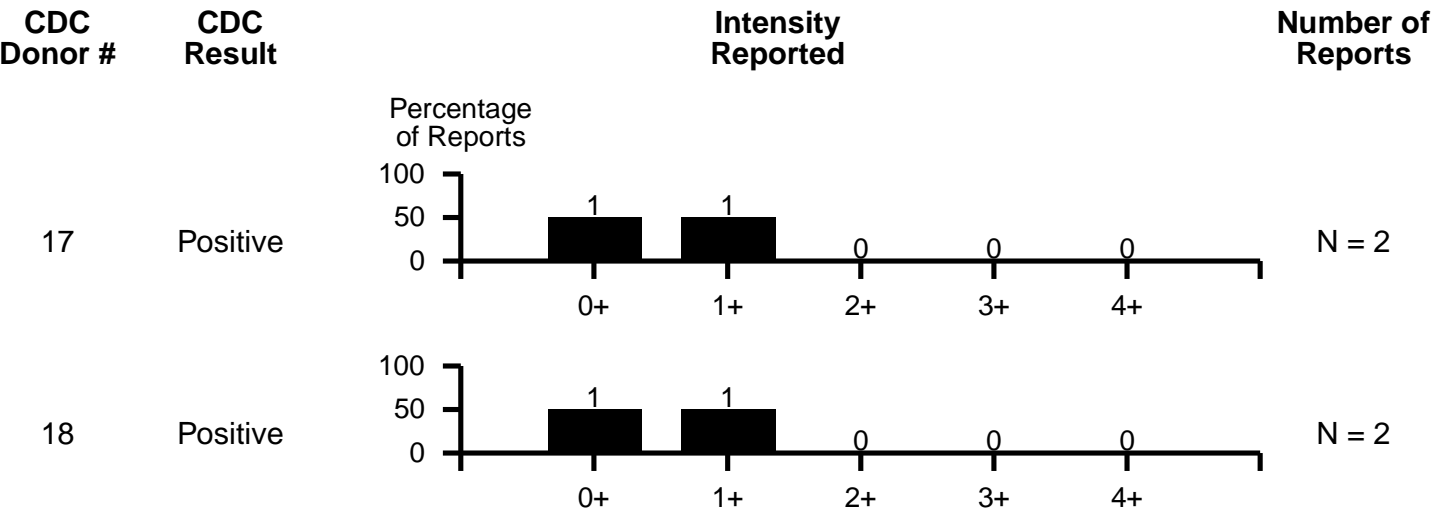


Figure 10. Types of 'Other' HIV test kits used and results reported by reference laboratories to the CDC for the January 8, 1996 shipment

