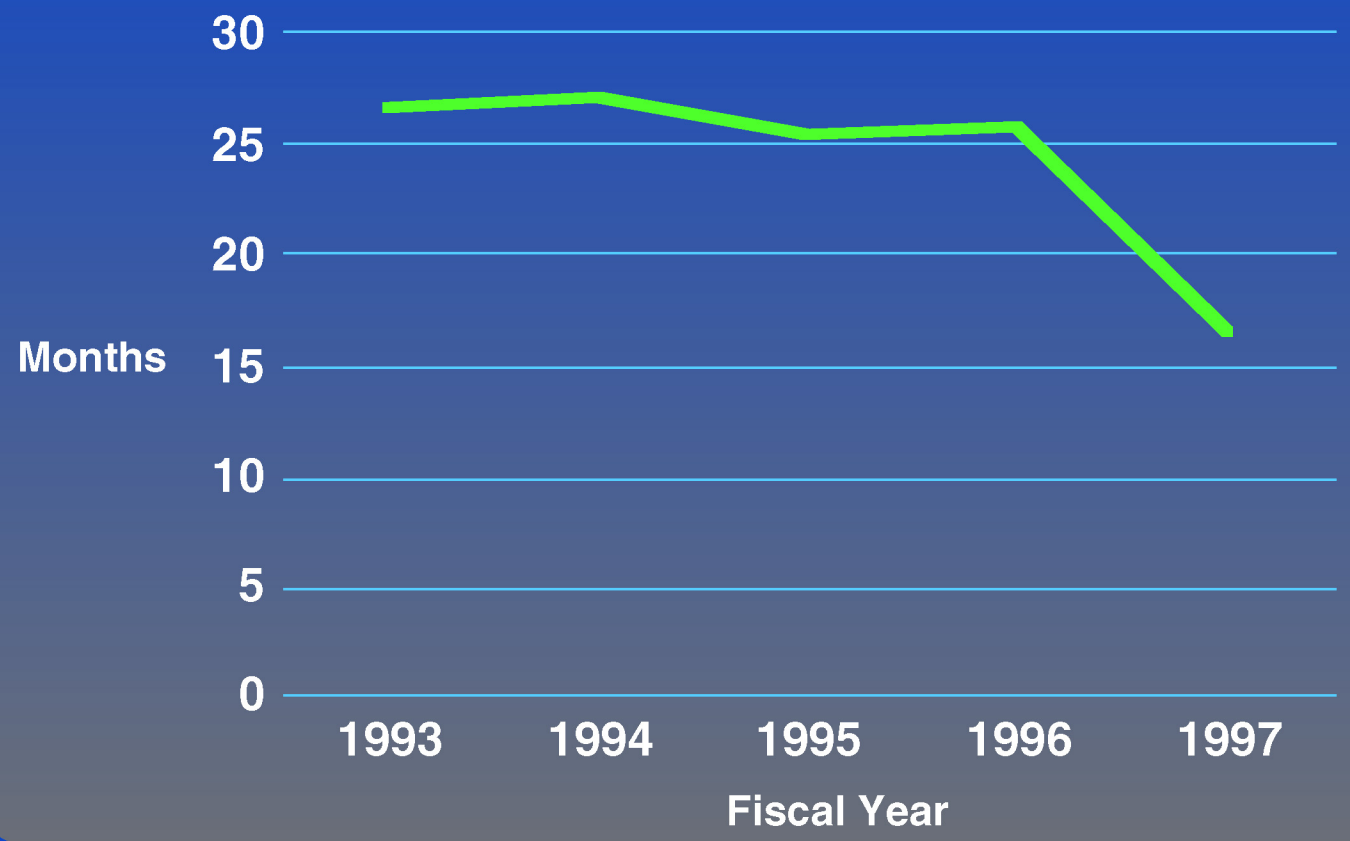Medical Devices
PMA Average Total Time