




Field-Portable Scanning Spectrofluorometer

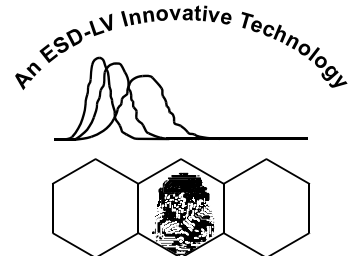

The Need

Field-portable instruments are available for the qualitative and quantitative evaluation of volatile organic compounds and non-volatile inorganic elements. Compounds that fall between these volatility extremes have received less attention in recent years. And yet these compounds comprise a surprising number of important contamination categories at Superfund and RCRA sites.

Polyaromatic hydrocarbons (PAHs) in complex mixtures such as oils, creosotes, and tars are found on numerous hazardous waste sites and, because of their high molecular weight, present special challenges to analytical chemists and instrument developers. These compounds have relatively high luminescence yields and, therefore, can be readily measured by spectrofluorometry.

A recent technology that is in the production prototype stage is the Field-Portable Scanning Spectrofluorometer (FPSS). It is a lightweight battery-operated instrument that has shown early

promise as a screening device for petroleum oils, PAHs and, especially, creosotes.

Creosote (wood preservation) and coal gasification sites are widespread, especially in the southeastern United States. These are complex sites that usually have various PAHs in addition to the creosotes. These compounds are currently quantified by gas chromatography but their tarlike composition makes them difficult to detect and destructive to columns and detectors. The development of a field-portable instrument to rapidly identify and quantify PAH mixtures, such as creosotes, oils, asphalts, or coal tars is an important step in filling a field analytical niche.

The FPSS prototype is ready for field demonstration and comparative studies. It is anticipated that the FPSS will provide a more rugged and less expensive alternative to traditional methods for screening PAHs.

The Use

Scientists working at the National Exposure Research Laboratory, Human Exposure Research Branch in Las Vegas (HERB-LV) have performed laboratory evaluations of the battery-operated FPSS developed by T. Vo-Dinh and his co-workers at Oak Ridge National Laboratory.^{2,4,5} Table 1 shows the physical characteristics of the instrument. The FPSS can perform emission and synchronous

The FPSS consists of three parts: a small suitcase-sized instrument that houses the optics and electronics, a battery pack, and a lap top computer used for instrument control, data storage and analysis. The spectral coverage of the instrument is 210-650 nm. The instrument parameters are chosen by the operator who uses the computer to control the instrument.

Table 1. Physical Characteristics of the Field-Portable Scanning Spectrofluorometer

	Size	Weight
Instrument	48 x 40 x 21 cm (18.5 x 11.5 x 8")	11.5 kg
Battery Pack	31 x 18 x 15 cm (12 x 7 x 6")	11.0 kg

wavelength scans. In the emission mode, relatively low detection limits are achieved (Table 2). The emission mode is useful for the determination of total PAHs or in identifying and classifying oils. In the synchronous mode, both the excitation and emission monochromators are scanned simultaneously with a constant wavelength offset. The advantage to synchronous mode is that it separates spectra of compounds with a different number of fused rings, sharpens spectra, and allows the relative amount of various PAH classes to be quantified.

Table 2. Limit of Detection (S/N = 3)

	Synchronous (cuvette)	Emission (cuvette)	Synchronous (fiber)
Perkin Elmer LS50 (laboratory instrument)	0.17*	0.02	24
FPSS prototype	3.5	0.55	1

The FPSS can be operated two ways: using a standard fluorescence cuvette cell or a bifurcated optical fiber. The optical fiber attachment is 2-meter long and allows direct screening of water samples. The cuvette can be used with liquid samples or extracts of soils. When the optical fiber attachment is used, care must be taken to avoid interference from light. This can be done by covering the sampling area with a black cloth.

The Limits

Some areas of concern exist relative to the successful operation of the FPSS in a field situation. The ruggedness of the optical components is crucial to the in situ applicability of the system. The unit was shipped from Oak Ridge National Laboratory to the HERB-LV without affecting the optical alignment or electronics. The instrument has been demonstrated to withstand normal handling in the laboratory. The instrument is ready to be demonstrated at a hazardous waste site.

be used with site-specific standards to quantify total oils or PAHs. It can be used to determine relative amounts of the PAH classes present. In rare instances, like spills of solvents or PAHs with very high fluorescent yields and sharp structures such as benzo-(a)pyrene, it can be used to detect and quantify identified PAHs. There is greater spectral separation capability when the instrument is operated in synchronous mode but lower detection limits can be achieved using the emission mode.

The FPSS is particularly suited to the classification or identification of oils or PAH compounds. It can also

The Status

Laboratory evaluations and research efforts have resulted in a draft fluorescence method for the analysis of PAHs which is in the final stages of acceptance by the American Society for Testing and Materials. A comparison of the optical fiber mode and the standard cuvette mode was performed on samples of anthracene in methanol. This study showed the cuvette mode to be 2-3 times more sensitive than the optical fiber mode.

types and sources. The FPSS proved its ability in a study comparing samples from an oil spill with samples of the source oil which were provided by the U.S. Coast Guard.

Synchronous luminescence has been demonstrated to be useful in characterizing crude and fuel oils. The technique can be used to produce spectral fingerprints for the identification of oil contamination

The FPSS has shown considerable promise for the classification and quantitation of PAH compounds and oily mixtures.^{1,3,6} The portable instrument has been evaluated at hazardous waste sites, where it compared well with standard methods in a well-planned experimental design. The development of the FPSS was sponsored by the HERB-LV and commercialization is being planned.

References

Amick, E. N., W. H. Engelmann, K. W. Brown, S. L. Wallace, C. J. Canfield, J. V. Fontana and R. D. Edmondson, "**Field Screening of Petroleum Hydrocarbons Using Synchronous Scanning Fluorescence Spectrometry.**" Presented at the Fifth International Symposium on Field Screening Methods for Hazardous Wastes and Toxic Chemicals, Las Vegas, NV, January 29-31, 1997, and published in the Proceedings of the Symposium.

Amick, E. N., J. E. Pollard, W. H. Engelmann, K. W. Brown, J. P. Alarie, W. Watts, T. Vo-Dinh, F. M. Akindele, and A. B. Crockett. "**Polycyclic Aromatic Hydrocarbon Pollutants From U. S. and Antarctic Sites Analyzed with Synchronous Fluorescence Spectrometry.**" Presented at Fourth International Symposium on Field Screening Methods for Hazardous Wastes and Toxic Chemicals, Las Vegas, NV, February 22-24, 1995, and published in the Proceedings of the Symposium.

Gerlach, C. L. (1996) New instrument brings PAH analysis to the field. *Environ. Sci. Technol.* 30(6) 252A-254A.

Alarie, J. P., W. E. Watts, D. R. Miller, G. J. Hyfantis, G. H. Peeler, W. H. Engelmann, and T. Vo-Dinh. "**Field Screening of Polycyclic Hydrocarbon Contamination in Soil Using a Portable Synchronous Scanning Spectrofluorometer.**" Presented at the International Conference on Environmental Monitors and Hazardous Waste Site Remediation, Munich, Germany, June 19-23, 1995, and published in the Proceedings of the Conference.

Amick, E. N., J. E. Pollard, W. H. Engelmann, and T. Vo-Dinh. "**In Situ Screening for PAHs with a Portable Spectrofluorometer at a Superfund Site Near Jackson, Tennessee.**" Presented at Innovate Site Characterization Technologies Section, 12th International Hazmat Conference, Philadelphia, PA, June 15-17, 1994, and published in the Conference Proceedings.

Engelmann, W. H., "Field Portable Monitor for PAHs" *TECH TRENDS*, The Applied Technologies Journal for Superfund Removals & Remedial Actions & RCRA Corrective Actions. U. S. EPA, Office of Solid Waste and Emergency Response, Washington, DC, EPA 542-N-95-001, Issue 19, March 1995, p. 2.

For Further

For further information about synchronous luminescence spectroscopy, contact:

For information about evaluating the FPSS at a hazardous waste site (Superfund or RCRA), contact:

Mr. William H. Engelmann
U.S. Environmental Protection Agency
National Exposure Research Laboratory
Human Exposure Research Branch
P.O. Box 93478
Las Vegas, NV 89193-3478
Phone: (702) 798-2664

Mr. J. Gareth Pearson, Director
Technology Support Center
U.S. Environmental Protection Agency
National Exposure Research Laboratory
Environmental Sciences Division
P.O. Box 93478
Las Vegas, NV 89193-3478
Phone: (702) 798-2270 • Fax: (702) 798-3146

The Technology Support Center fact sheet series is developed and written by Clare L. Gerlach, Lockheed Martin, Las Vegas.

