File Names

File #	Original File Name
1	ENVCAN_STIFS_WBZ_JRB_EC+OC_PARTISOL_2001_07_V1.csv

	Principal Investigator Namelast		File Contents Descriptionshort	
Data Exchange Standard Version	first	Principal Investigator Affiliation	long	Sampling Interval As Reported in Main Table
NARSTO 2002/05/28 (2.301)	, ,	· · · · · · · · · · · · · · · · · · ·		8 h day/16 h night
		Meteorological Service of Canada	Organic Carbon mass	
			concentration	

Sampling Frequency Of Data in Main Table	Quality Control Level	Organization Acronym	Organization Name	Data Usage Acknowledgement	Study Or Network Acronym
2 times per day	1	ENVCAN_MSC	Environment	Environment Canada,	ENVCAN_STIFS
			CanadaMeteorological	Meteorological Service of	
			Service of Canada	Canada, 4905 Dufferin St.,	
				Toronto, Ont. M3H 5T4	

				Co-investigator Namelast	
Study Or Network Name	Country Code	State Or Province Code	Principal Investigator Contact Information	first	Co-investigator Affiliation
Environment CanadaSupersite Transboundary Intensive Field Study	CA		Environment Canada, Meteorological Service of Canada, 4905 Dufferin St., Toronto, Ont. M3H 5T4	None ; None	None

Name And Affiliation Of Person Who Generated This File	Date Of Last Modification To Data In Main Table	Name And Version Of Software Used To Create This File
Greg Skelton, SKELTON TECHNICAL SERVICES INC	2003/01/24	MS Excel/2002

•	Date This File Generated	
format And Version	archive Version Number	Table Explanation Of Zero Or Negative Values
None ; 0		Blank corrections are performed after samples are compared to the DL and flagged accordingly. Only the variables that have a mean blank concentration that is >5% of the mean air concentration (in units of ug/filter) are corrected by subtracting the mean blank concentration (in ug/filter). In some cases this results in final concentrations in ug/m^3 that are negative or less than the stated detection limit (in ug/m^3). Such samples are not flagged as BDL because on a ug/filter basis before blank correction they were above the detection limit. The user may also choose to classify this samples as BDL.

Table Explanation Of Reported Detection Limit Values	Table Explanation Of Reported Uncertainty	Table User Note	Table User Note2	Table User Note3	Table User Note4
Detection limits (DL) are based upon 3*SD of field blanks in ug/filter. Non blank-corrected laboratory analysis results in ug/filter for each sample are	no uncertainty reported	None	None		
compared to this DL to determine if the sample is BDL and then flagged					
accordingly (V1 means BDL).					

Table Name	Table Focus
EC+OC_mass	Surfacefixed

Site Information

		State			Sampling height	Ground elevation	
Site ID	Name	Province code	Latitude: decimal degree	Longitude: decimal degree	above ground (m)	above sea level (m)	Site land use
STIFCAQUWBZ_	St. Anicet	ON	45.11667	-74.28333	2.0	49.0	Agricultural


				Co-incident		Lat
Site ID	Site location setting	Measurement start date	Measurement end date	measurements	Study site ID	Ion accuracy
STIFCAQUWBZ_	Rural	2001/06/30	2001/08/03	CO, NO, NOy, global radiation (RF1), VOC polar and non-polar		

Flag: NARSTO	Description				
H1	Historical data that have not been assessed or validated				
M1	Missing value because no value is available				
M2	Missing value because invalidated by data originator				
	Missing value because invalidated by Data Originator				
	Missing value because invalidated by data originator				
V0	Valid value				
V1	Valid value but comprised wholly or partially of below detection limit data				
V2	Valid estimated value				
V3	Valid interpolated value				
V4	Valid value despite failing to meet some QC or statistical criteria				
V5	Valid value but qualified because of possible contamination (e.g., pollution source, laboratory contamination source)				
V6	Valid value but qualified due to non-standard sampling conditions				
	Valid value but qualified due to non-standard sampling conditions (e.g., instrument malfunction, sample handling)				
	Valid value but qualified due to non-standard sampling conditions				
V7	Valid value but set equal to the detection limit (DL) because the measured value was below the DL				

NAtChem Time Series Plot 21SEP2004

Site ID: STIFCAQUWBZ_ Variable name: Carbon: elemental (EC) Units: ug/m3 Sampling interval: 8 h day/16 h night
Sampling frequency: 2 times per day Observation type: Particles Particle diameter--lower bound (UM): Undetermined
Particle diameter--upper bound (UM): 2.5 Field sampling or measurement principle: Single filter Medium: Quartz
Inlet type: Impactor--virtual/concentrator Laboratory analytical method: Thermooptical transmission Sample preparation: Thermal desorption
Blank Correction: Blank corrected Volume standardization: 25 deg. C; 1 atmosphere Sampling Height above ground (m): 2
Instrument name and model number: Rupprecht and Patashnik Partisol-Plus 2025D Measurement principal investigator: Jeffrey Brook
Detection Limit: Varies--see Detection lim


Site Name: St. Anicet, Latitude: 45.11667 deg. Longitude: -74.28333 deg. Start Date: 2001-06-30 End Date: 2001-08-03

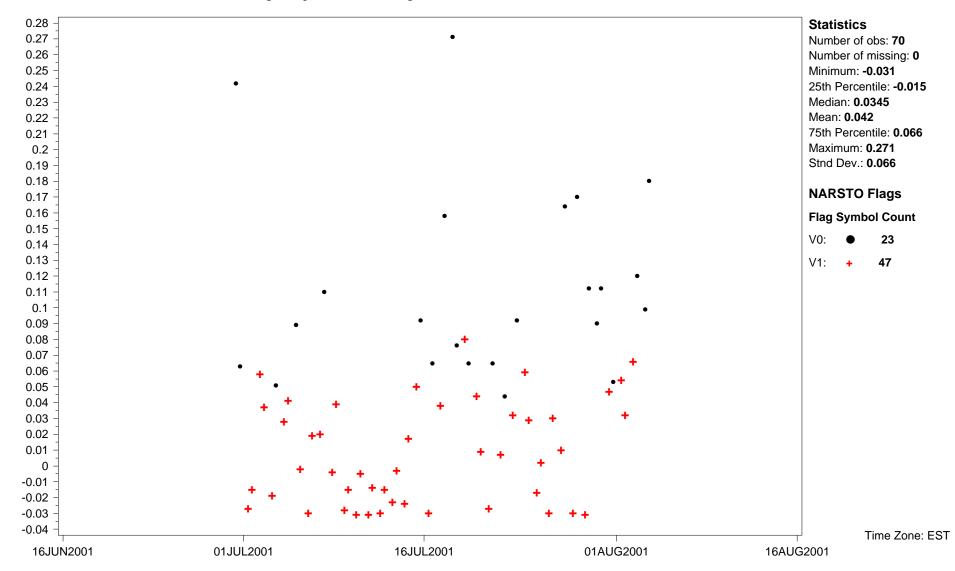

NAtChem Time Series Plot 21SEP2004

Site ID: STIFCAQUWBZ_ Variable name: Carbon: organic (OC) Units: ug/m3 Sampling interval: 8 h day/16 h night Sampling frequency: 2 times per day
Observation type: Particles Particle diameter--lower bound (UM): Undetermined Particle diameter--upper bound (UM): 2.5
Field sampling or measurement principle: Single filter Medium: Quartz Inlet type: Impactor--virtual/concentrator
Laboratory analytical method: Thermooptical transmission Sample preparation: Thermal desorption Blank Correction: Blank corrected
Volume standardization: 25 deg. C; 1 atmosphere Sampling Height above ground (m): 2
Instrument name and model number: Rupprecht and Patashnik Partisol-Plus 2025D Measurement principal investigator: Jeffrey Brook
Detection Limit: Varies--see Detection lim


Site Name:St. Anicet, Latitude:45.11667 deg. Longitude:-74.28333 deg. Start Date:2001-06-30 End Date:2001-08-03

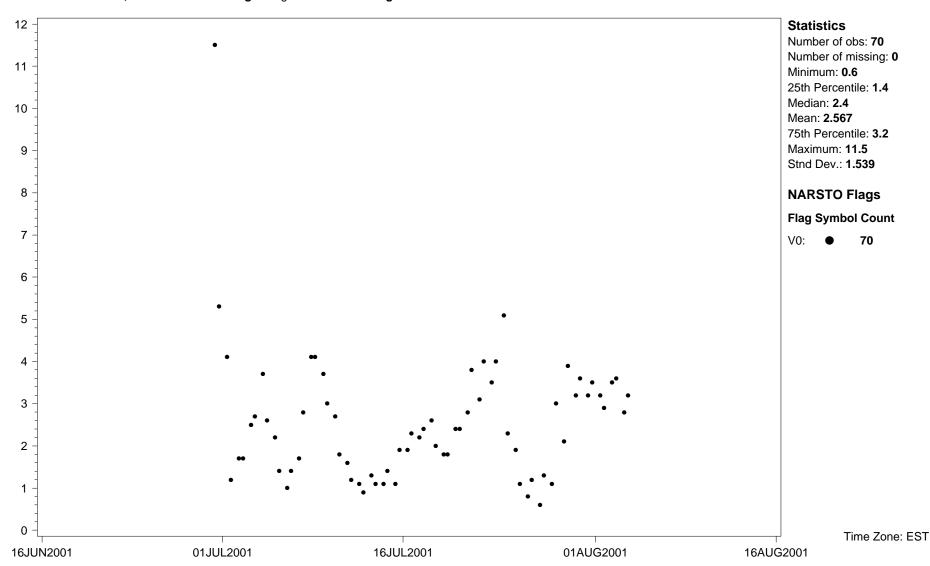

NAtChem Time Series Plot 219EP2004

Site ID: STIFCAQUWBZ_ Variable name: Carbon: organic (OCX2) Units: ug/m3 Sampling interval: 8 h day/16 h night
Sampling frequency: 2 times per day Observation type: Particles Particle diameter--lower bound (UM): Undetermined
Particle diameter--upper bound (UM): 2.5 Field sampling or measurement principle: Single filter Medium: Quartz
Inlet type: Impactor--virtual/concentrator Laboratory analytical method: Thermooptical transmission Sample preparation: Thermal desorption
Blank Correction: Blank corrected Volume standardization: 25 deg. C; 1 atmosphere Sampling Height above ground (m): 2
Instrument name and model number: Rupprecht and Patashnik Partisol-Plus 2025D Measurement principal investigator: Jeffrey Brook
Detection Limit: Varies--see Detection lim

Site Name: St. Anicet, Latitude: 45.11667 deg. Longitude: -74.28333 deg. Start Date: 2001-06-30 End Date: 2001-08-03

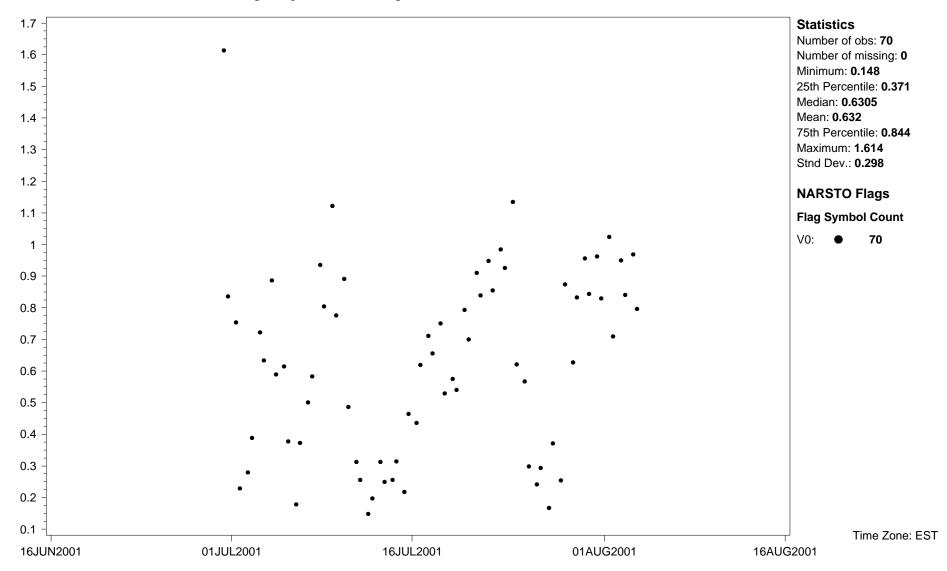

NAtChem Time Series Plot 21SEP2004

Site ID: STIFCAQUWBZ_ Variable name: Sample: total volume Units: m3 Sampling interval: 8 h day/16 h night Sampling frequency: 2 times per day Observation type: Flow Field sampling or measurement principle: Mass flow controller Volume standardization: 25 deg. C; 1 atmosphere Sampling Height above ground (m): 2 Instrument name and model number: Rupprecht and Patashnik Partisol-Plus 2025D Measurement principal investigator: Jeffrey Brook

Site Name: St. Anicet, Latitude: 45.11667 deg. Longitude: -74.28333 deg. Start Date: 2001-06-30 End Date: 2001-08-03

