


Hepatitis C Virus (HCV) Infection Testing for Diagnosis

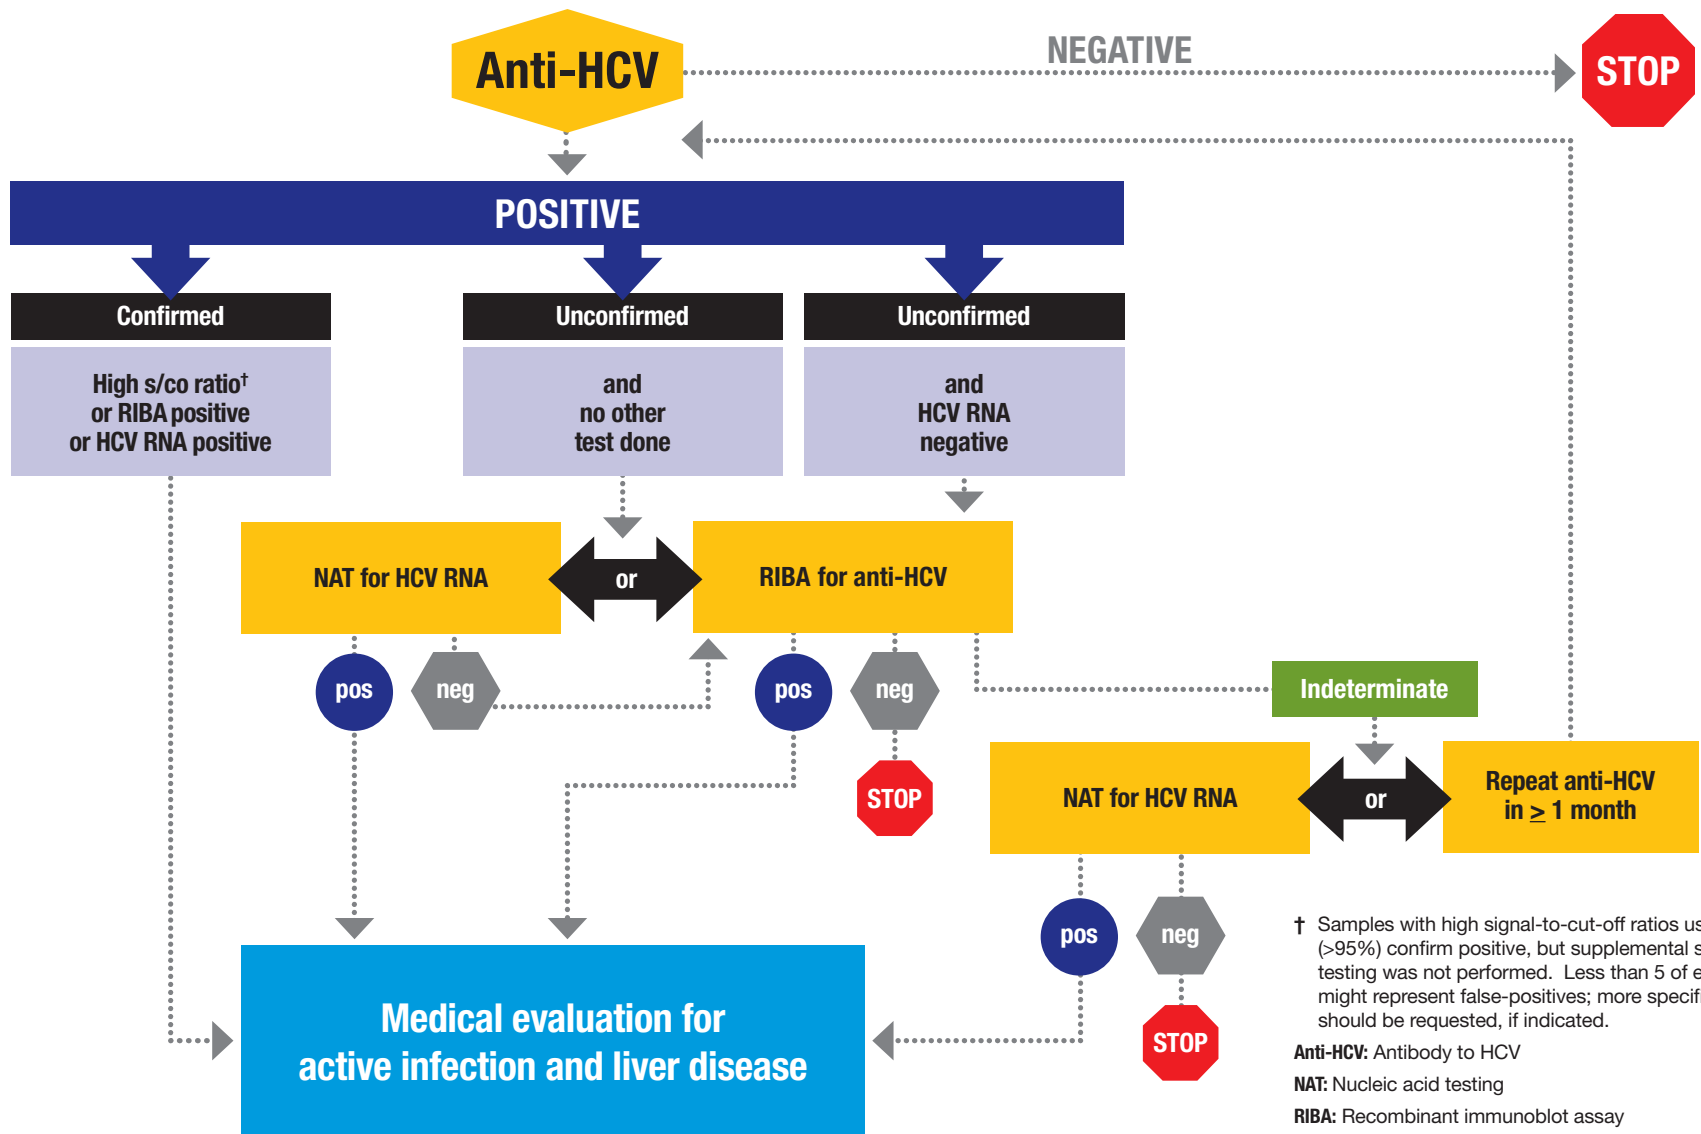

† Samples with high signal-to-cut-off ratios usually (>95%) confirm positive, but supplemental serologic testing was not performed. Less than 5 of every 100 might represent false-positives; more specific testing should be requested, if indicated.

Anti-HCV: Antibody to HCV

NAT: Nucleic acid testing

RIBA: Recombinant immunoblot assay

RNA: Ribonucleic acid



DEPARTMENT OF HEALTH & HUMAN SERVICES
Centers for Disease Control and Prevention

Division of Viral Hepatitis

