

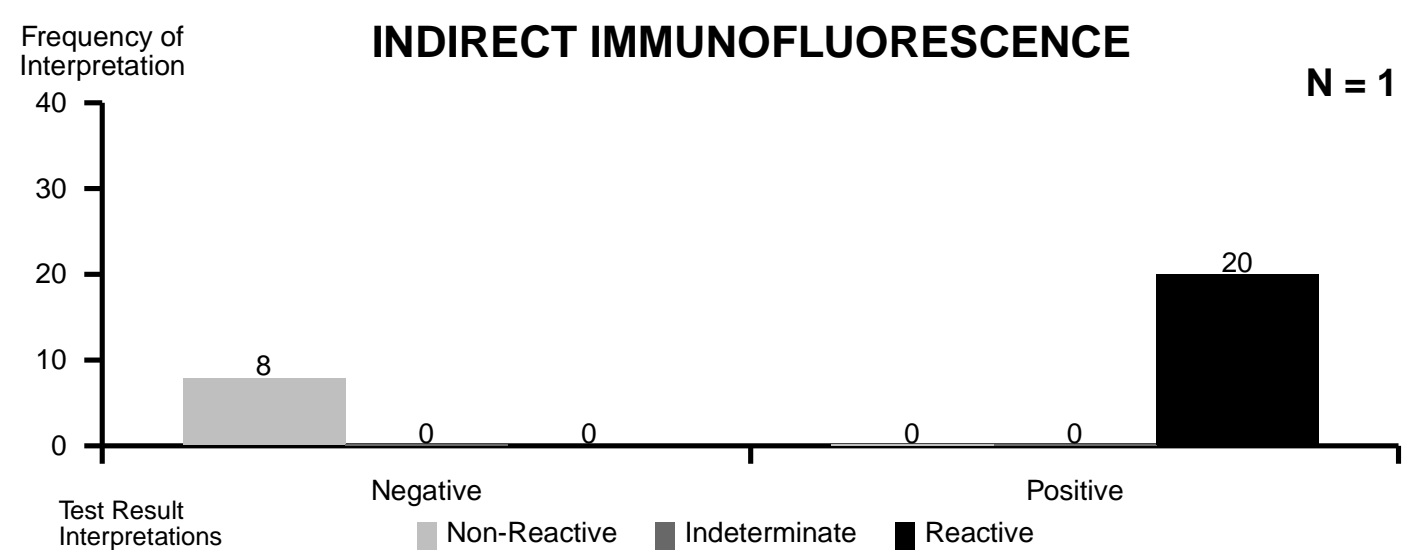
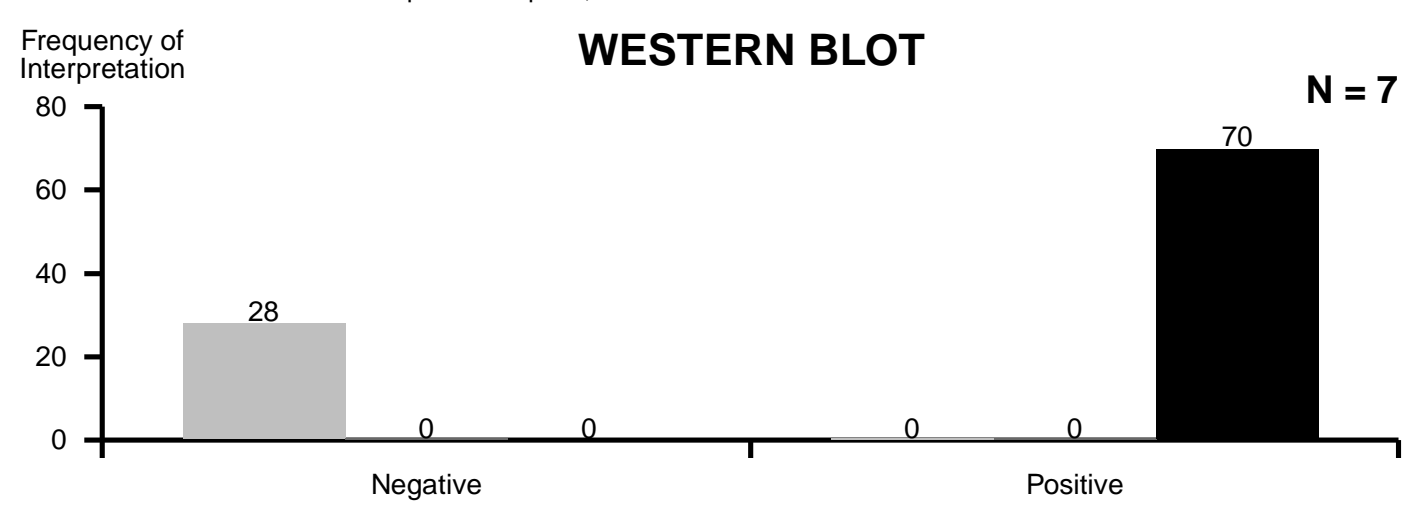



**Figure 1. Frequency of HTLV-I/II antibody test result interpretations, by sample type (reactivity), for the enzyme immunoassay (EIA), Western blot (WB), and indirect immunofluorescence (IIF), reported by reference laboratories for the April 15, 1996 shipment**

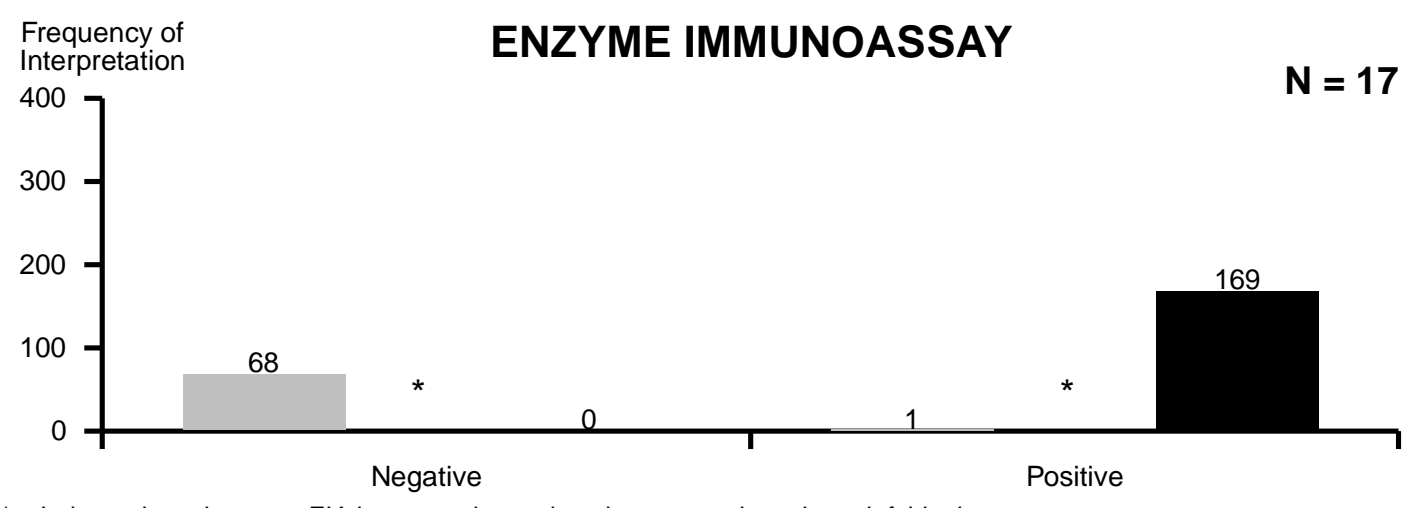




**Figure 2. Percentage of HTLV-I/II reference laboratories, by laboratory type, that reported results to the CDC for the April 15, 1996 shipment**

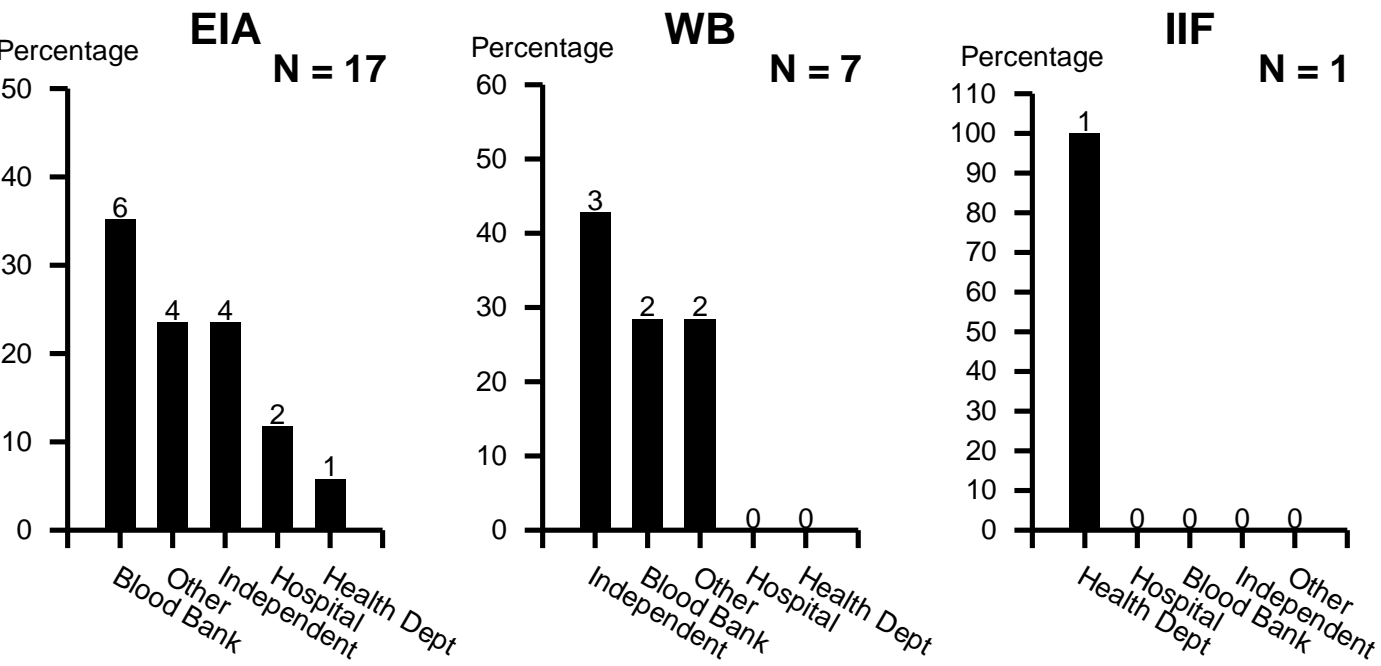



**Figure 3. Combination of HTLV-I/II tests reported by reference laboratories for the April 15, 1996 shipment**

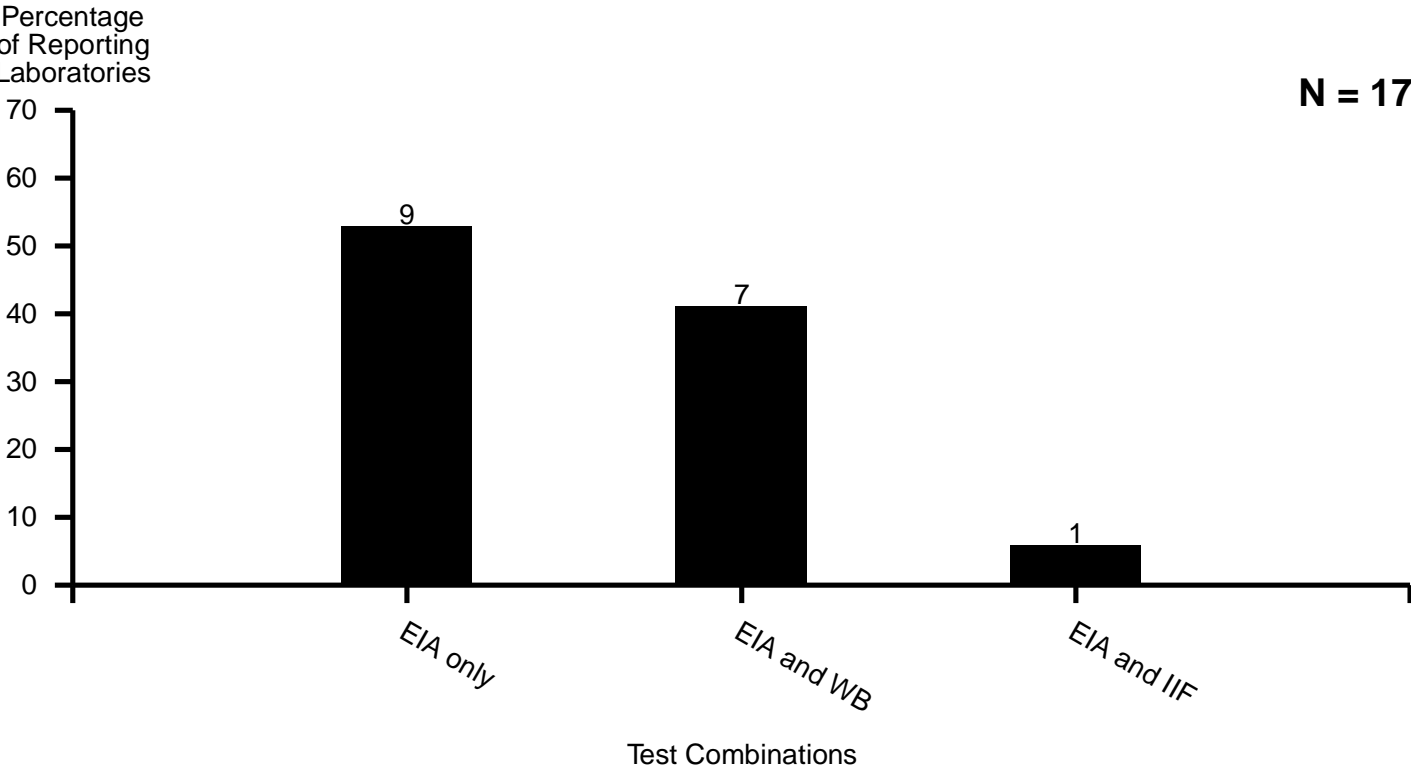

**Figure 4. Types of HTLV-I/II kits used for enzyme immunoassay, Western blot, and indirect immunofluorescence, as reported by reference laboratories to the CDC for the April 15, 1996 shipment**

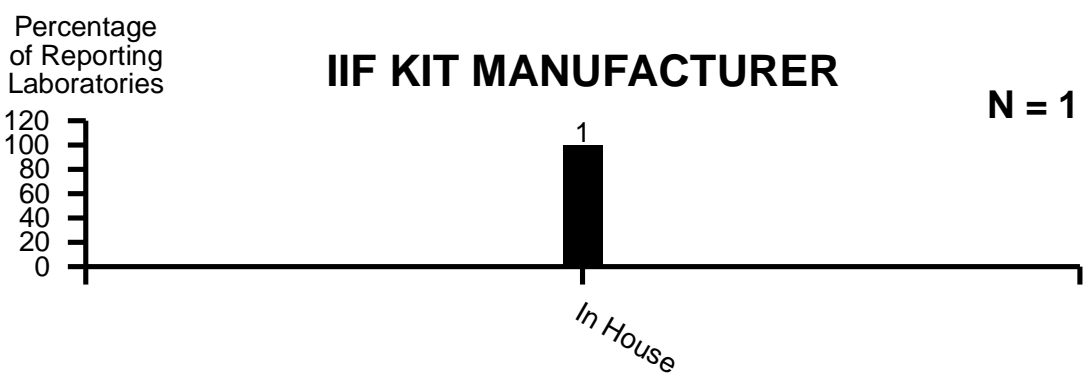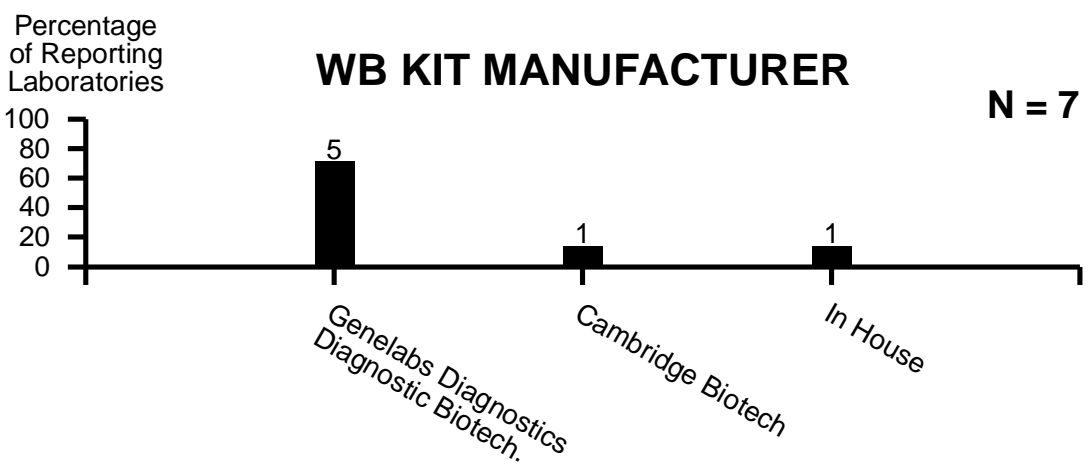
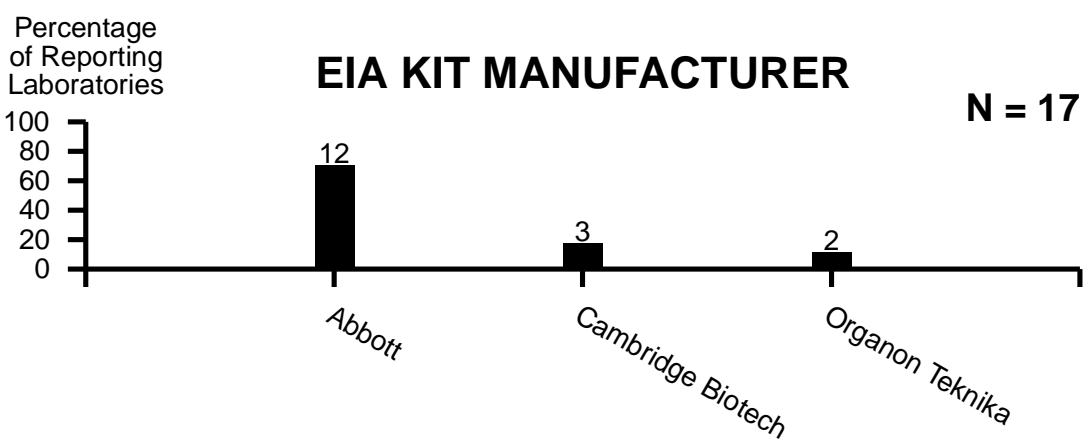


**Figure 5. Enzyme immunoassay HTLV-I/II results, by kit manufacturer, reported by reference laboratories for the April 15, 1996 shipment**

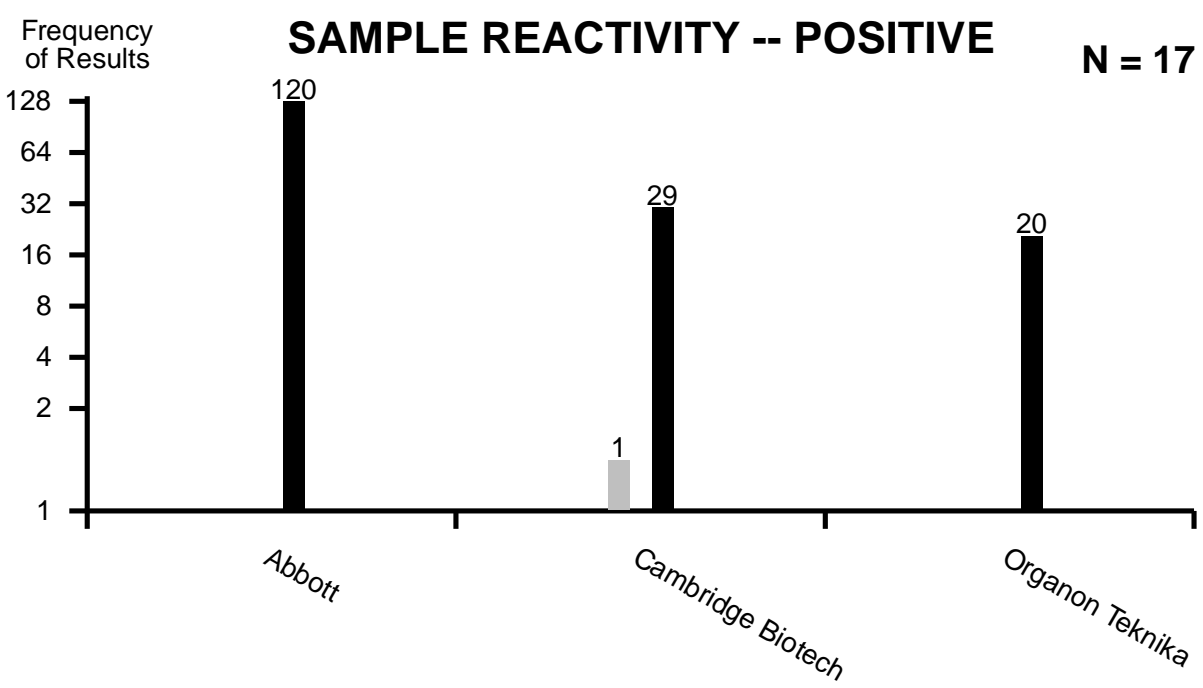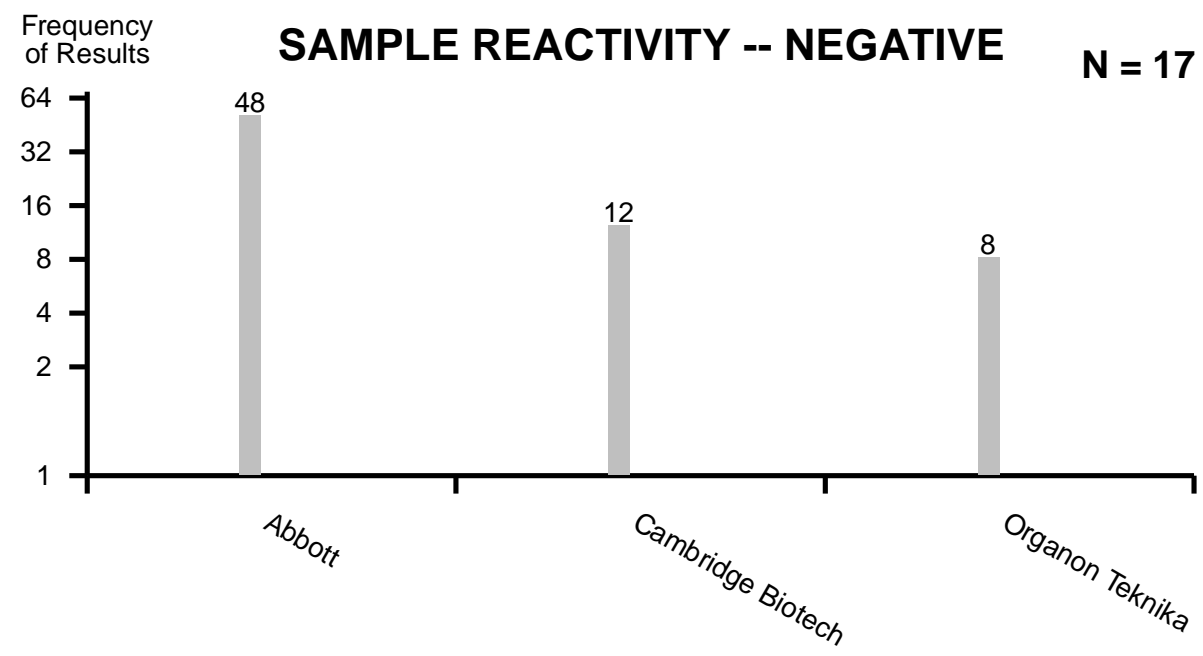



Test Result Interpretations ■ Non-Reactive ■ Reactive

**Figure 6. Western blot HTLV-I/II results, by kit manufacturer, reported by reference laboratories for the April 15, 1996 shipment**

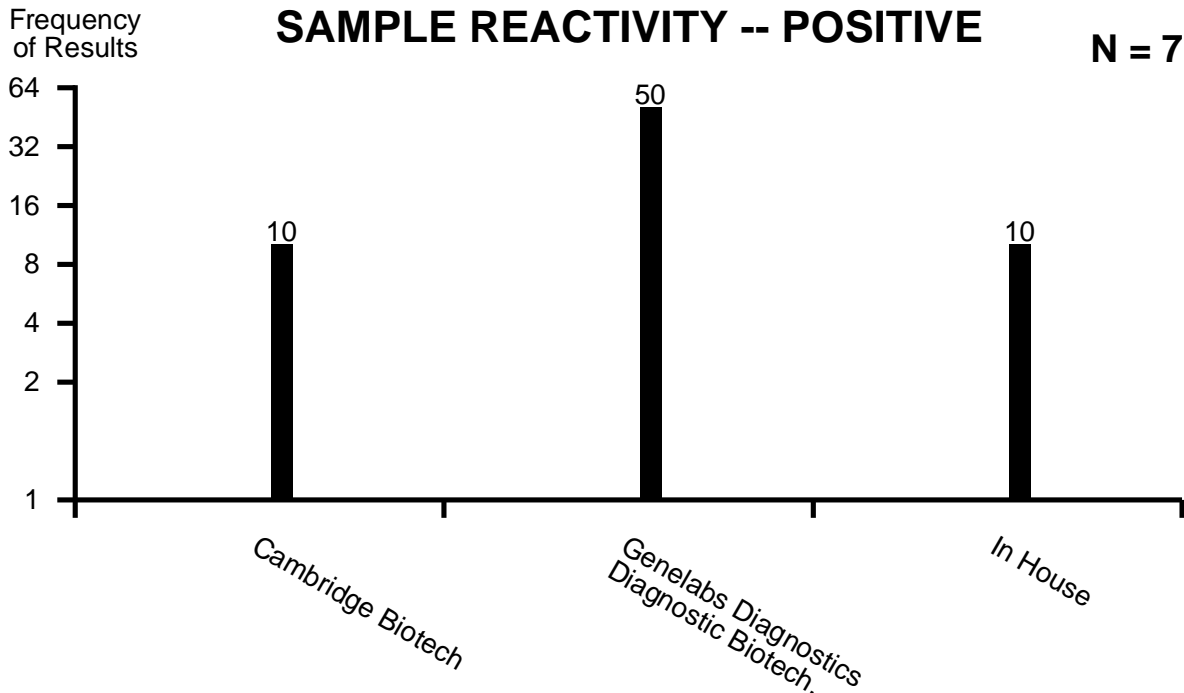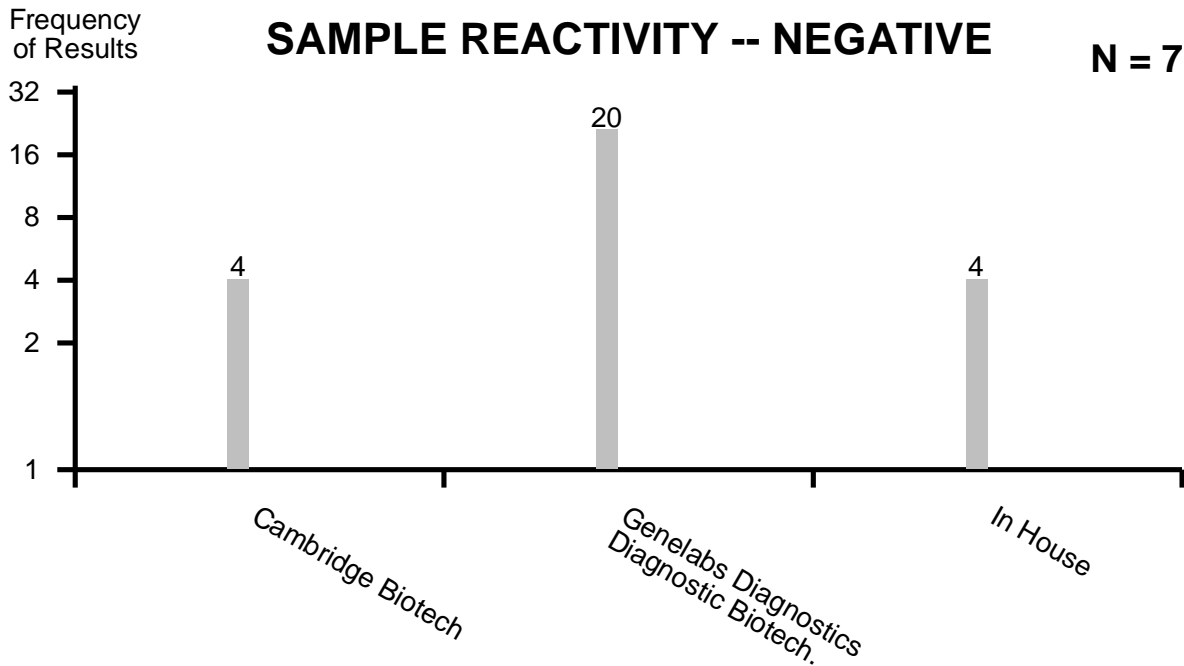

Test Result Interpretations ■ Non-Reactive ■ Indeterminate ■ Reactive


**Figure 7. Indirect immunofluorescence HTLV-I/II results, by kit manufacturer, reported by reference laboratories for the April 15, 1996 shipment**

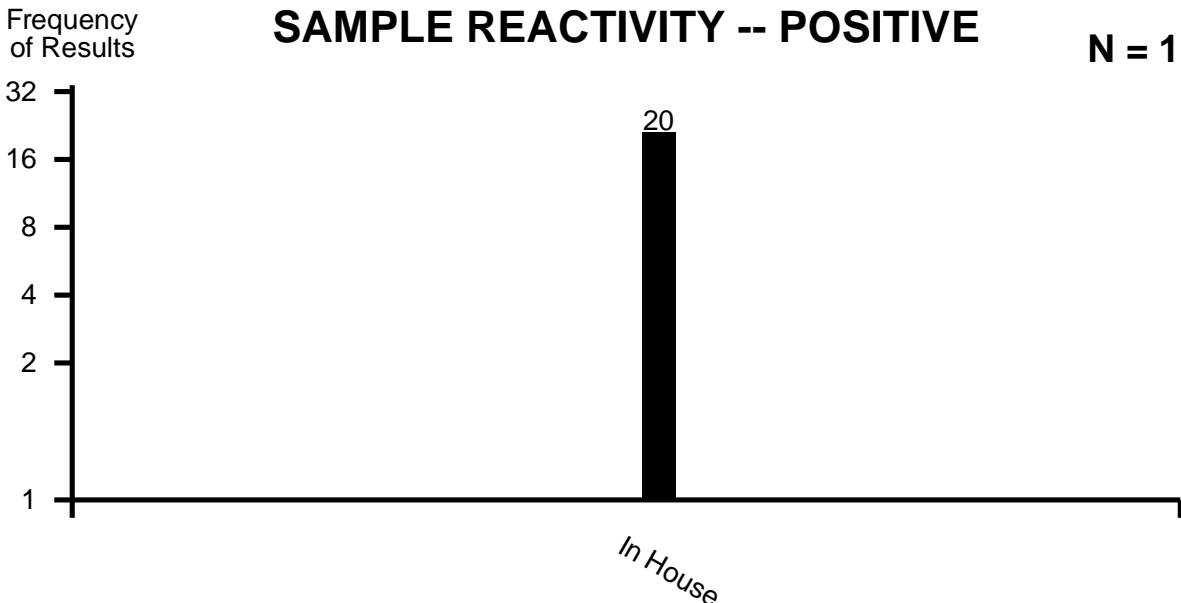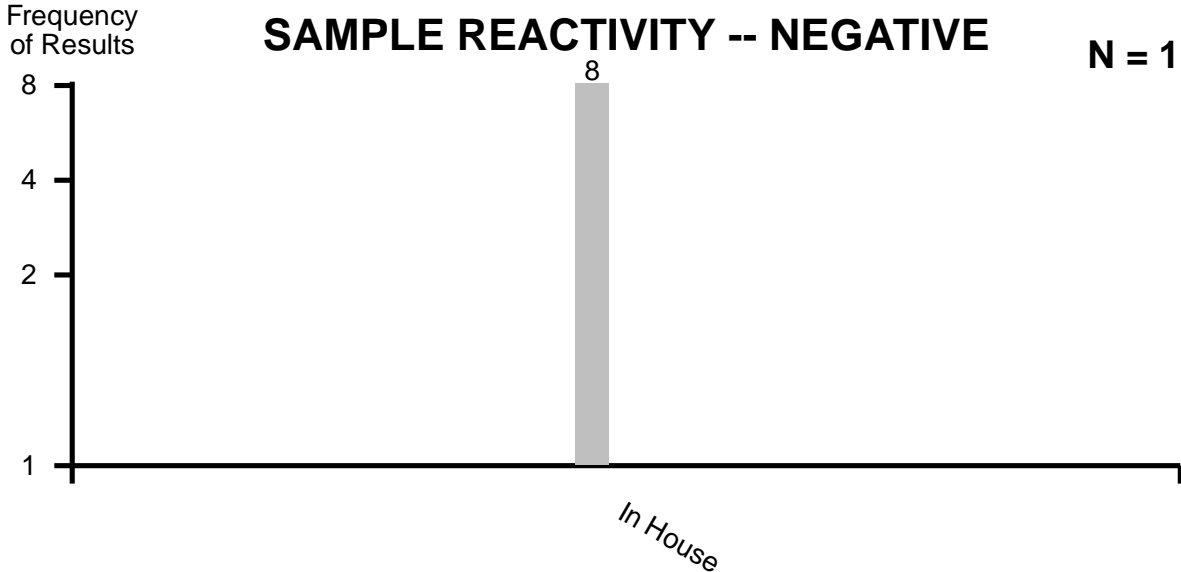


Test Result Interpretations

- Non-Reactive
- Indeterminate
- Reactive

**Figure 8. Western blot HTLV-I/II band patterns reported to CDC by reference laboratories for the April 15, 1996 shipment**

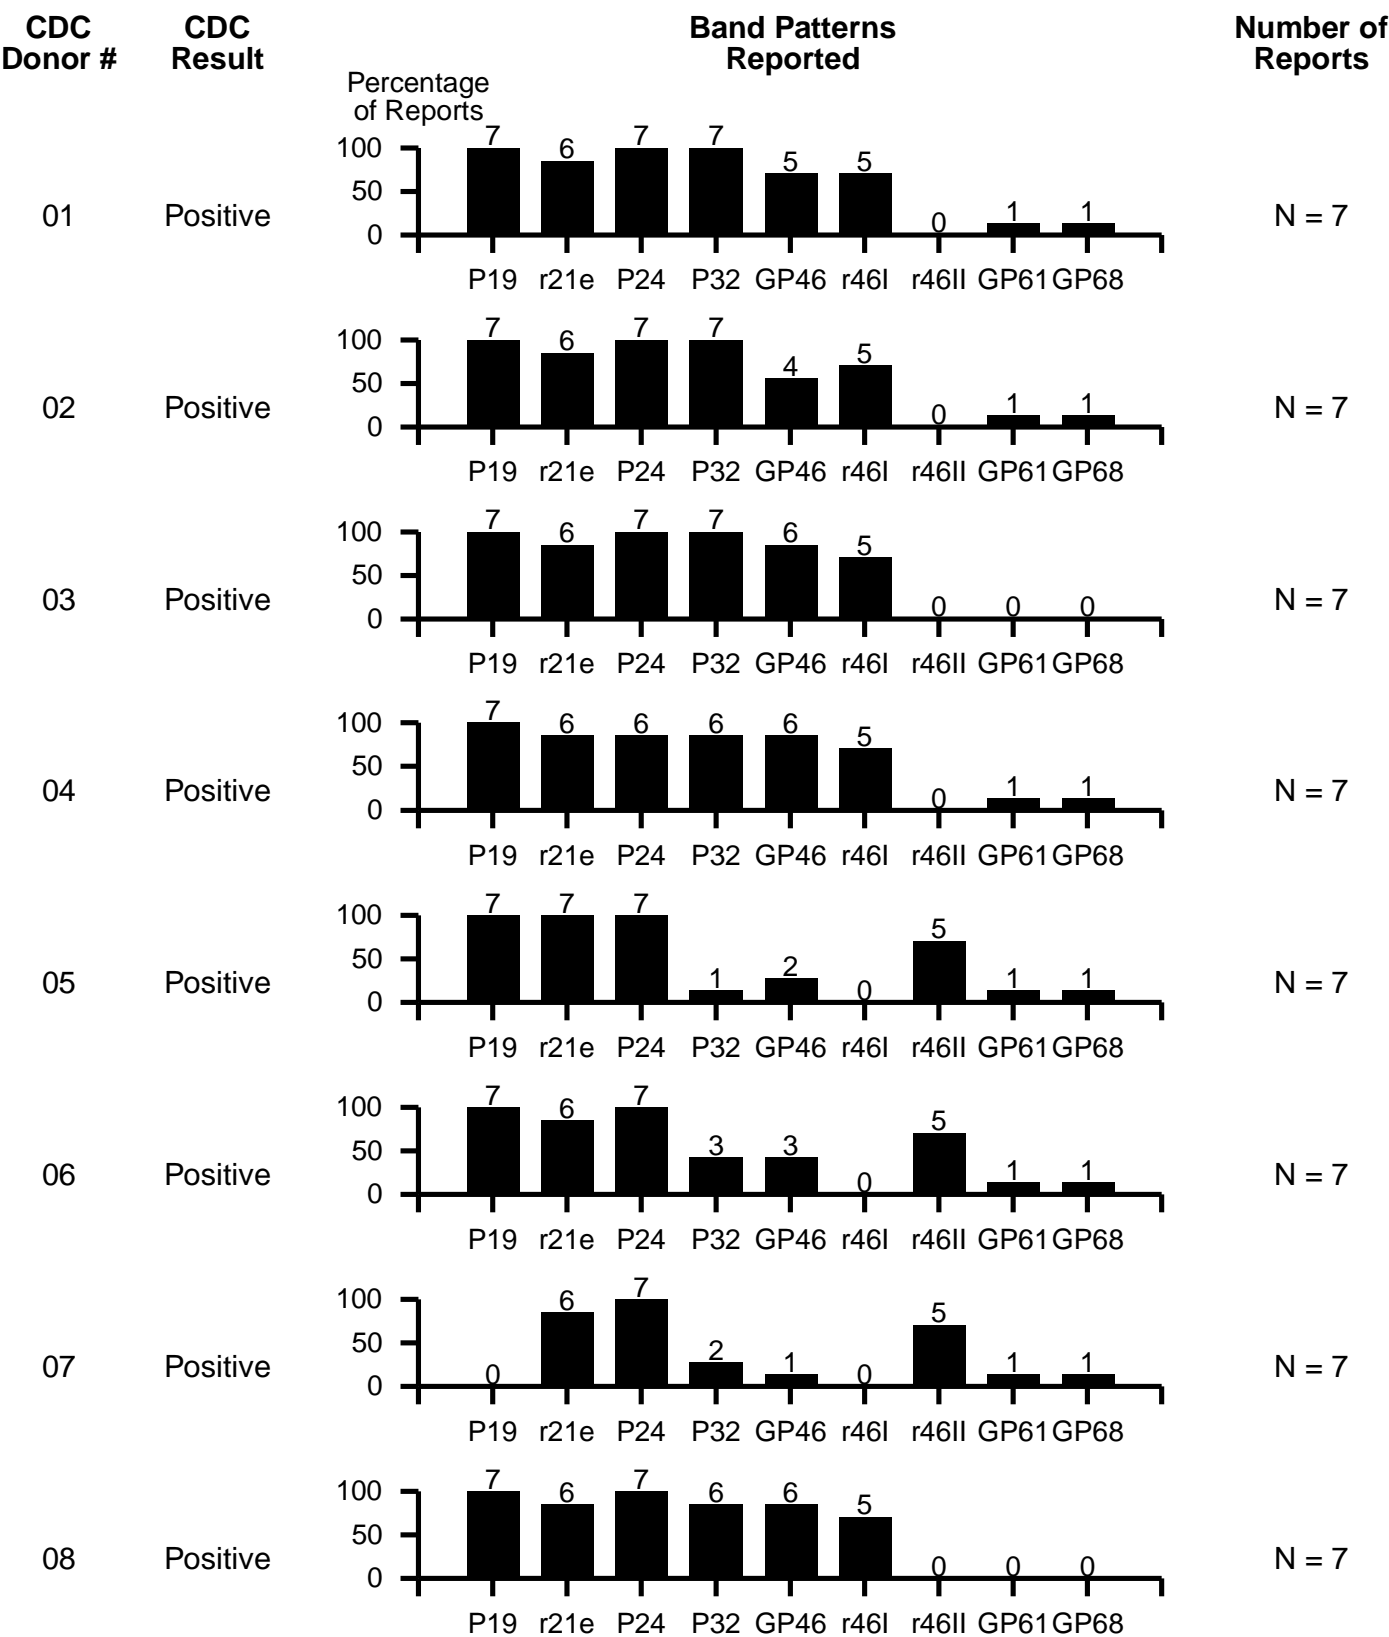


**Figure 8. Western blot HTLV-I/II band patterns reported to CDC by reference laboratories for the April 15, 1996 shipment**

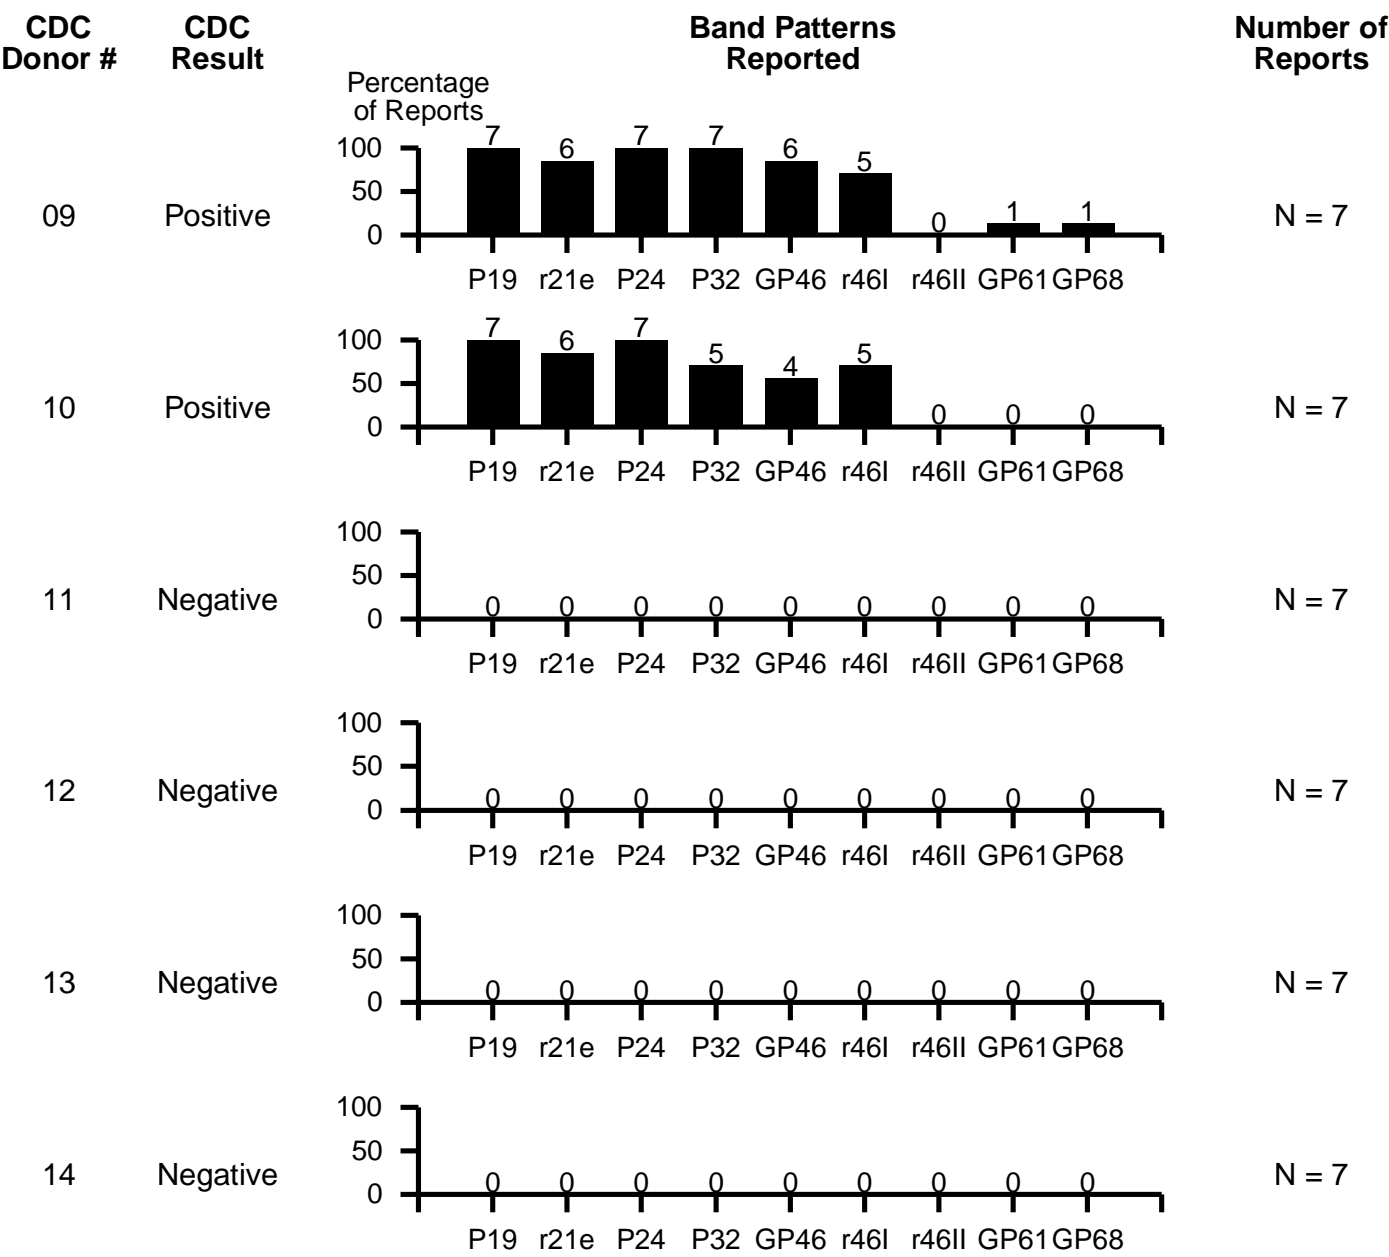







**Figure 9. Fluorescence intensity patterns, of HTLV-I/II-infected cells, for IIF results reported to CDC by reference laboratories for the April 15, 1996 shipment**

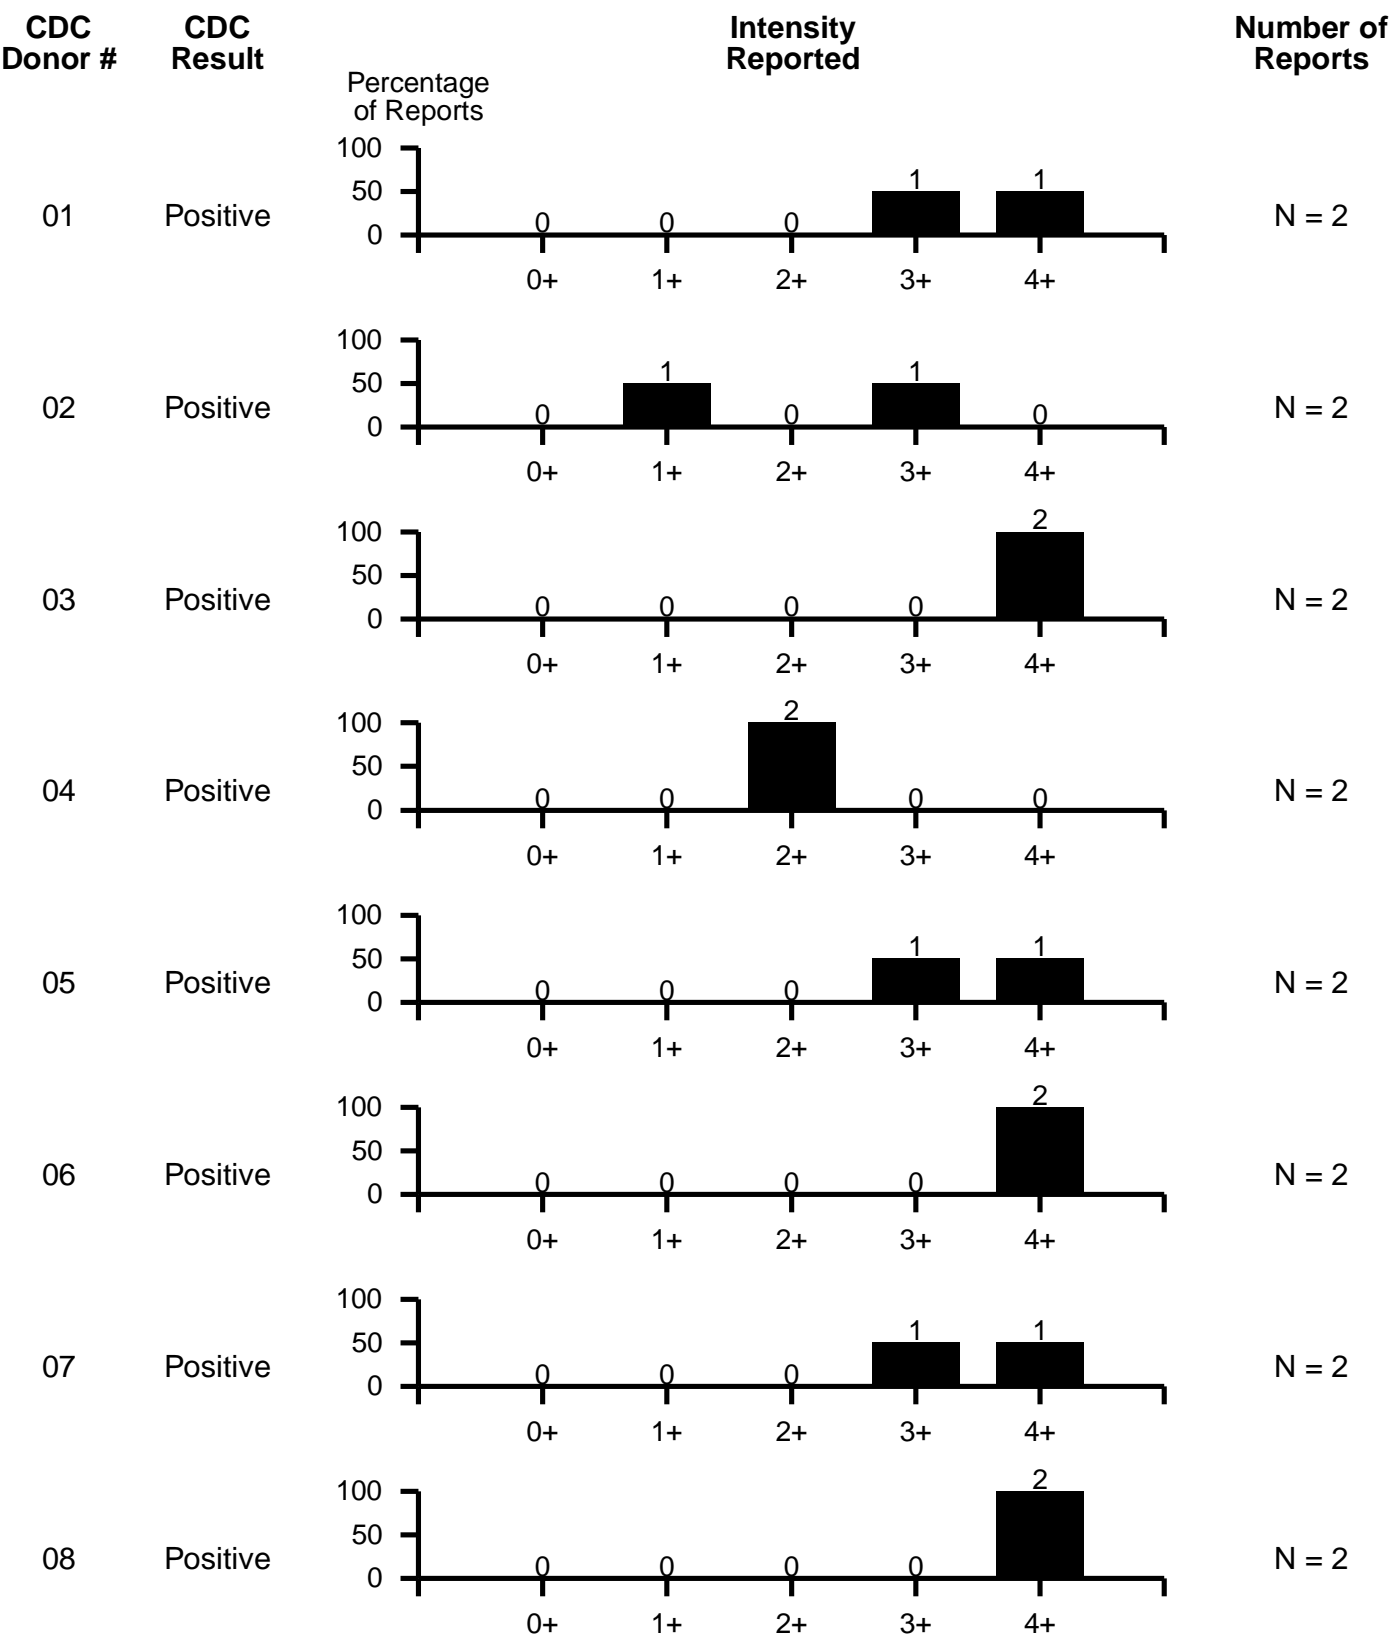

**Figure 9. Fluorescence intensity patterns, of HTLV-I/II-infected cells, for IIF results reported to CDC by reference laboratories for the April 15, 1996 shipment**

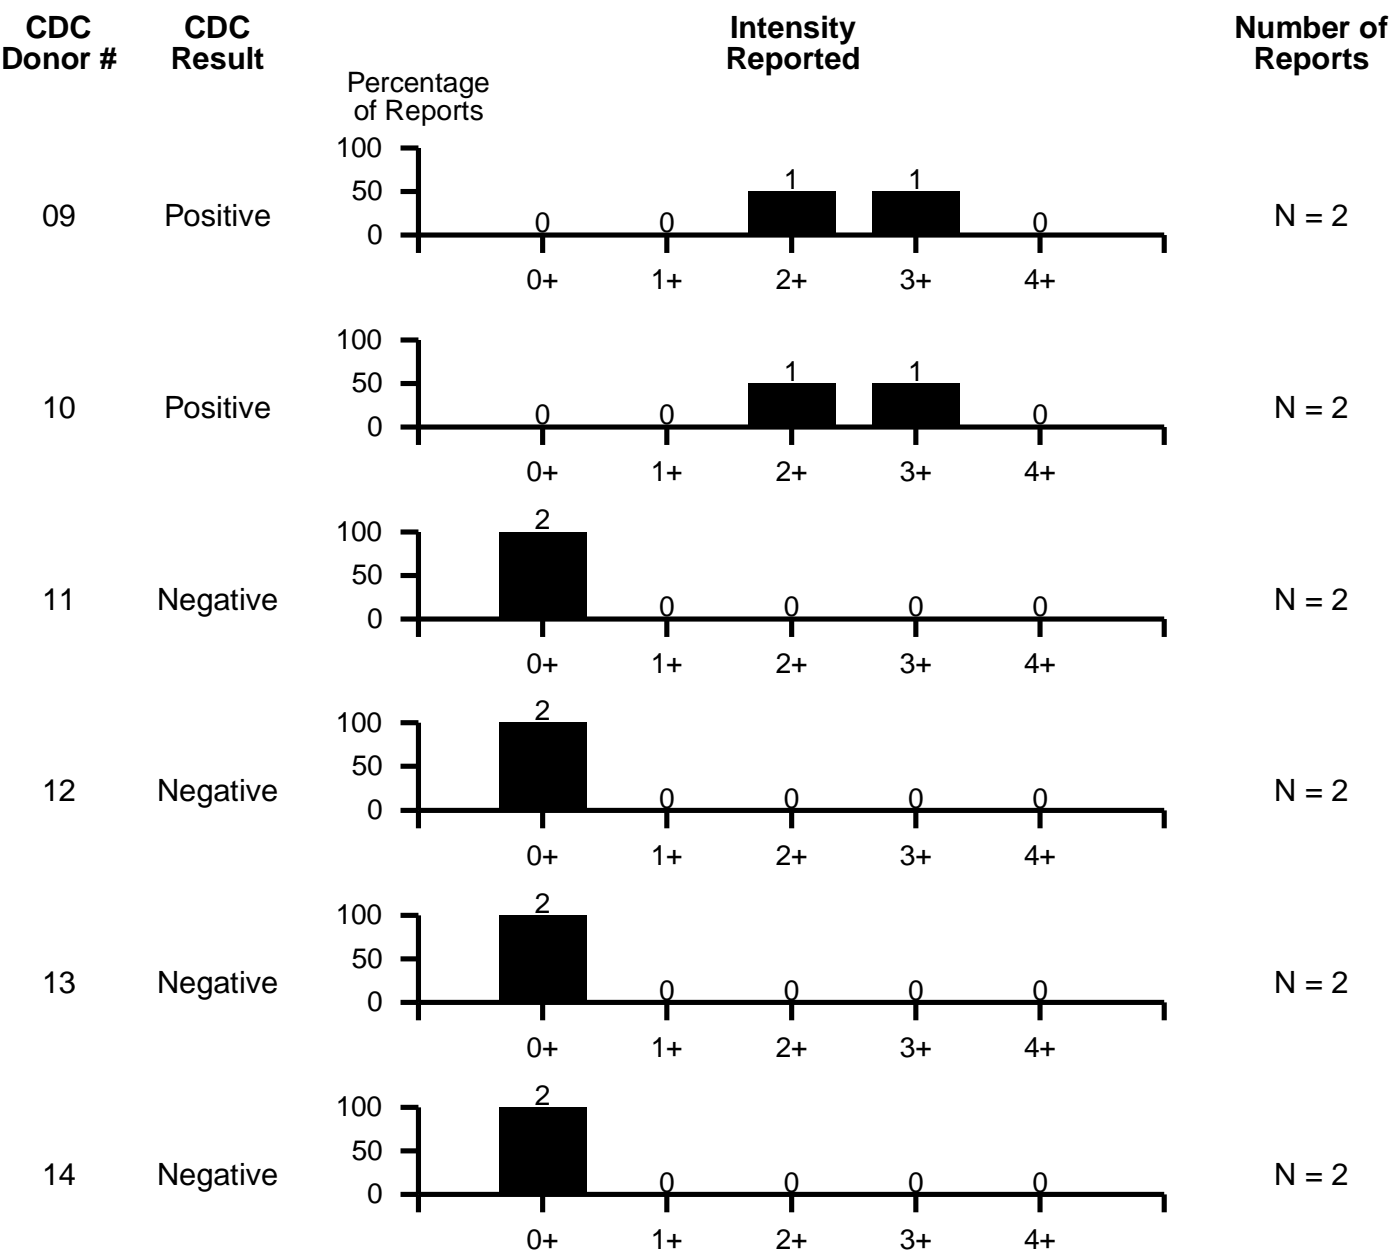

**Figure 10. Types of 'Other' HTLV test kits used and results reported by reference laboratories to the CDC for the April 15, 1996 shipment**

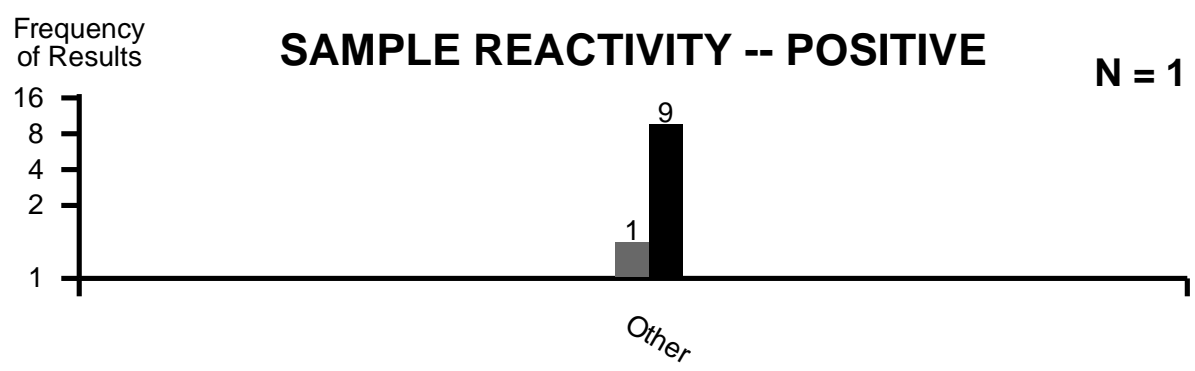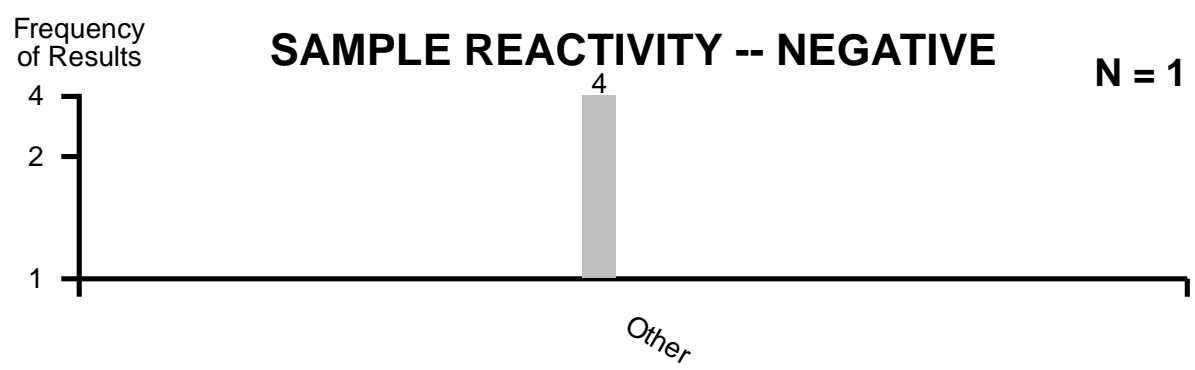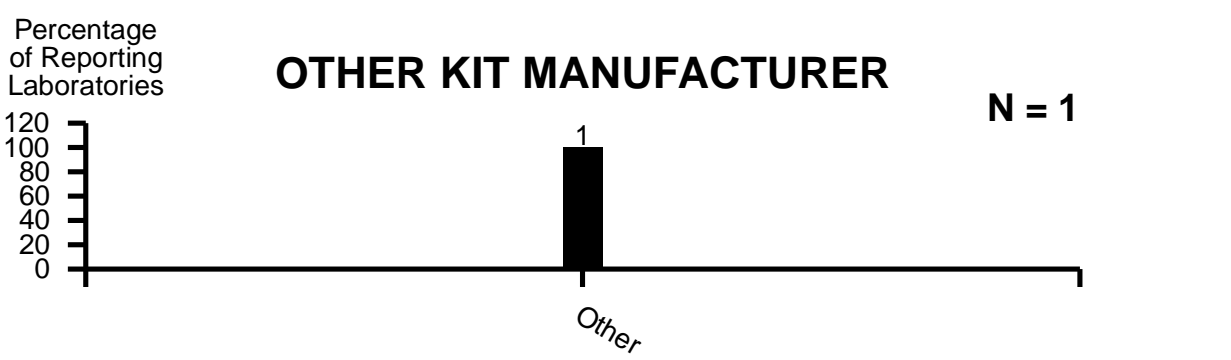

Test Result Interpretations:  Non-Reactive  Indeterminate  Reactive